Print of window 38: Current Chromatogram(s)
Data File : D:\DATA\02112021\16- -KD.D
Sample Name : AE-00053-10ML

AccuStandard®
Leader in Analytical Reference Standards

==========

Acq. Operator : SYSTEM Seq. Line : 1
Acq. Instrument : LCMS-1 Location : P1-E5
Injection Date : 2/11/2021 1:58:39 PM Inj : 1
Inj Volume : 1.000 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 4.000 µl
Method : C:\CHEM32\1\METHODS\Purity195_315.M
Last changed : 5/8/2020 11:20:44 AM by SYSTEM
Method Info : Operator: Oraganic QC lab
Gradient Method Starting @ 100 % Water/0 % Acetonitrile to 0 % Water/100 % Acetonitrile in 13 min, then 3 min at 100/0, post-run time 2 min. Flow rate:0.3 ml /min, column Zorbax Eclipse Plus C-18, 2.1x50 mm, 1.8 micron particule size. Agilent 1290 Infinity II LC system, Agilent 6120 Quadrople MS Detector. No UV Reference.

Additional Info : Peak(s) manually integrated

Current Chromatogram(s)

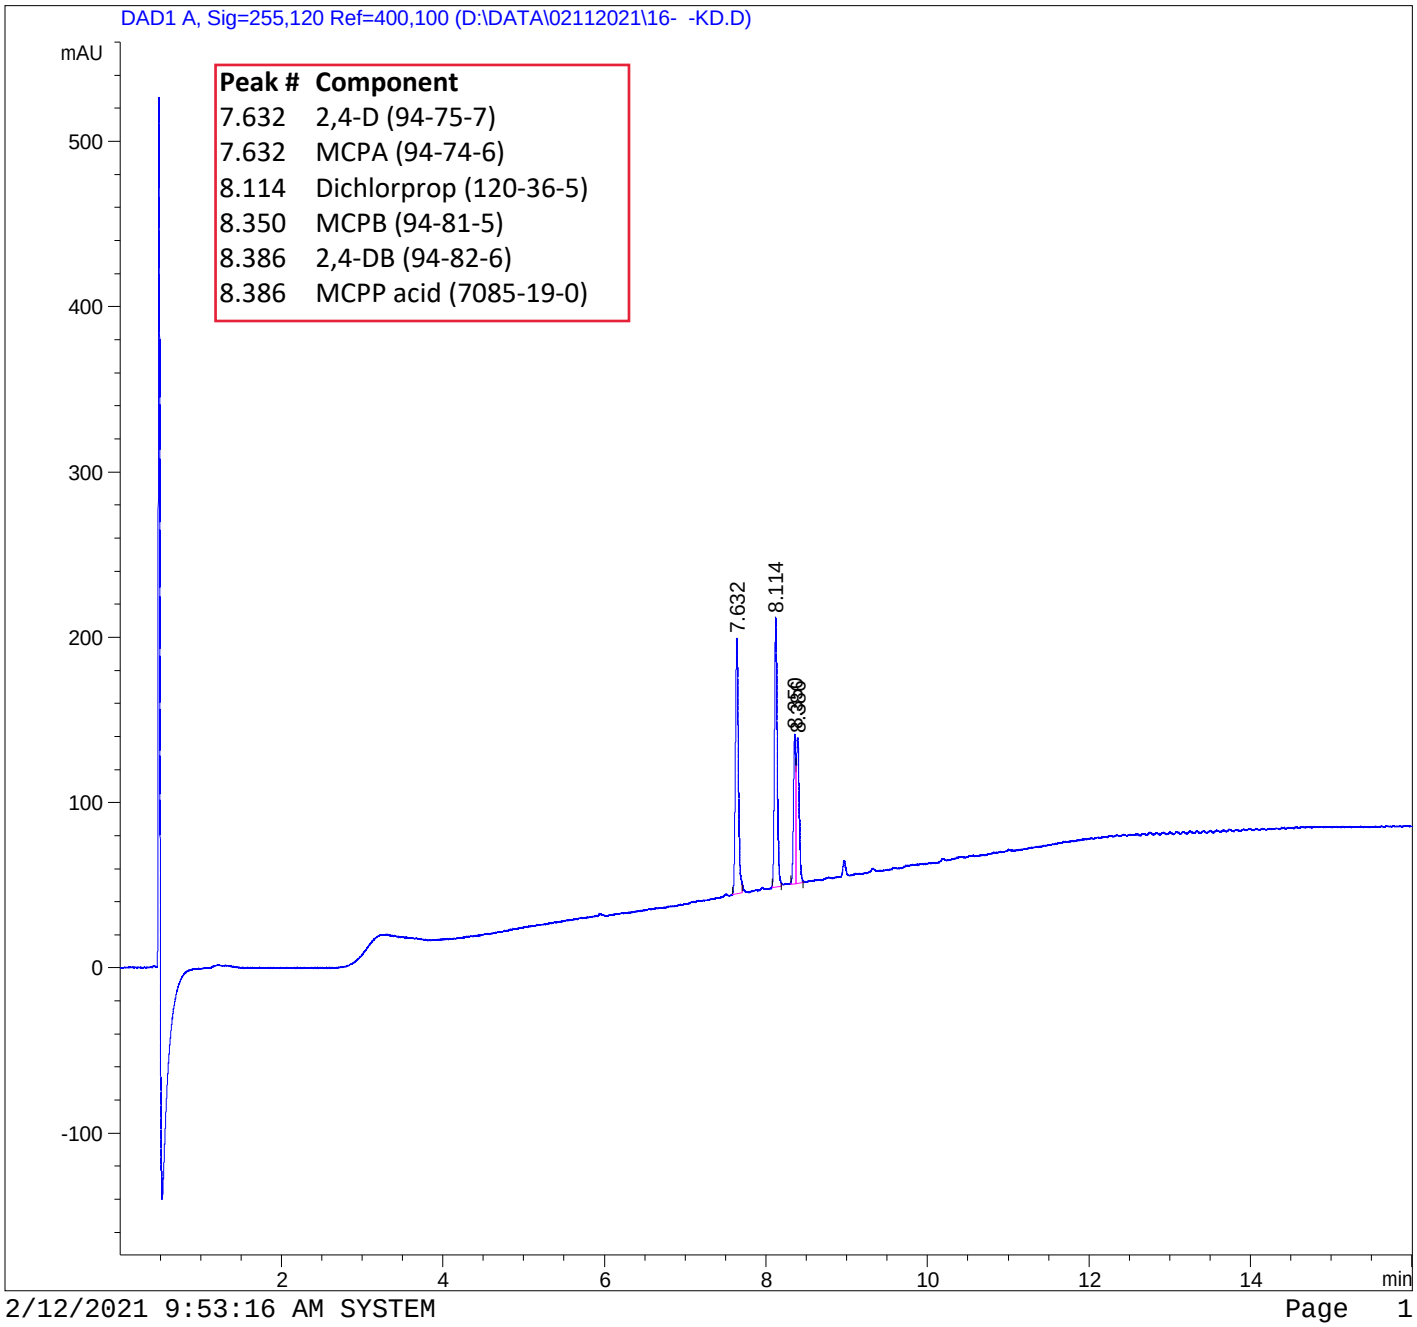

Peak #	Component
7.632	2,4-D (94-75-7)
7.632	MCPA (94-74-6)
8.114	Dichlorprop (120-36-5)
8.350	MCPB (94-81-5)
8.386	2,4-DB (94-82-6)
8.386	MCPP acid (7085-19-0)