AccuStandard®
Leader in Analytical Reference Standards

Column: DB-5, 30m, 0.25 ID, 0.25um
Oven Program: 100c, 1m, 30c/min to 320c, final 2min.
GC Parameters: Pulsed split 40psi 0.5m, 10psi constant flow
Split 20:1, 1ul inj.; GC/MS; INJ 250c.
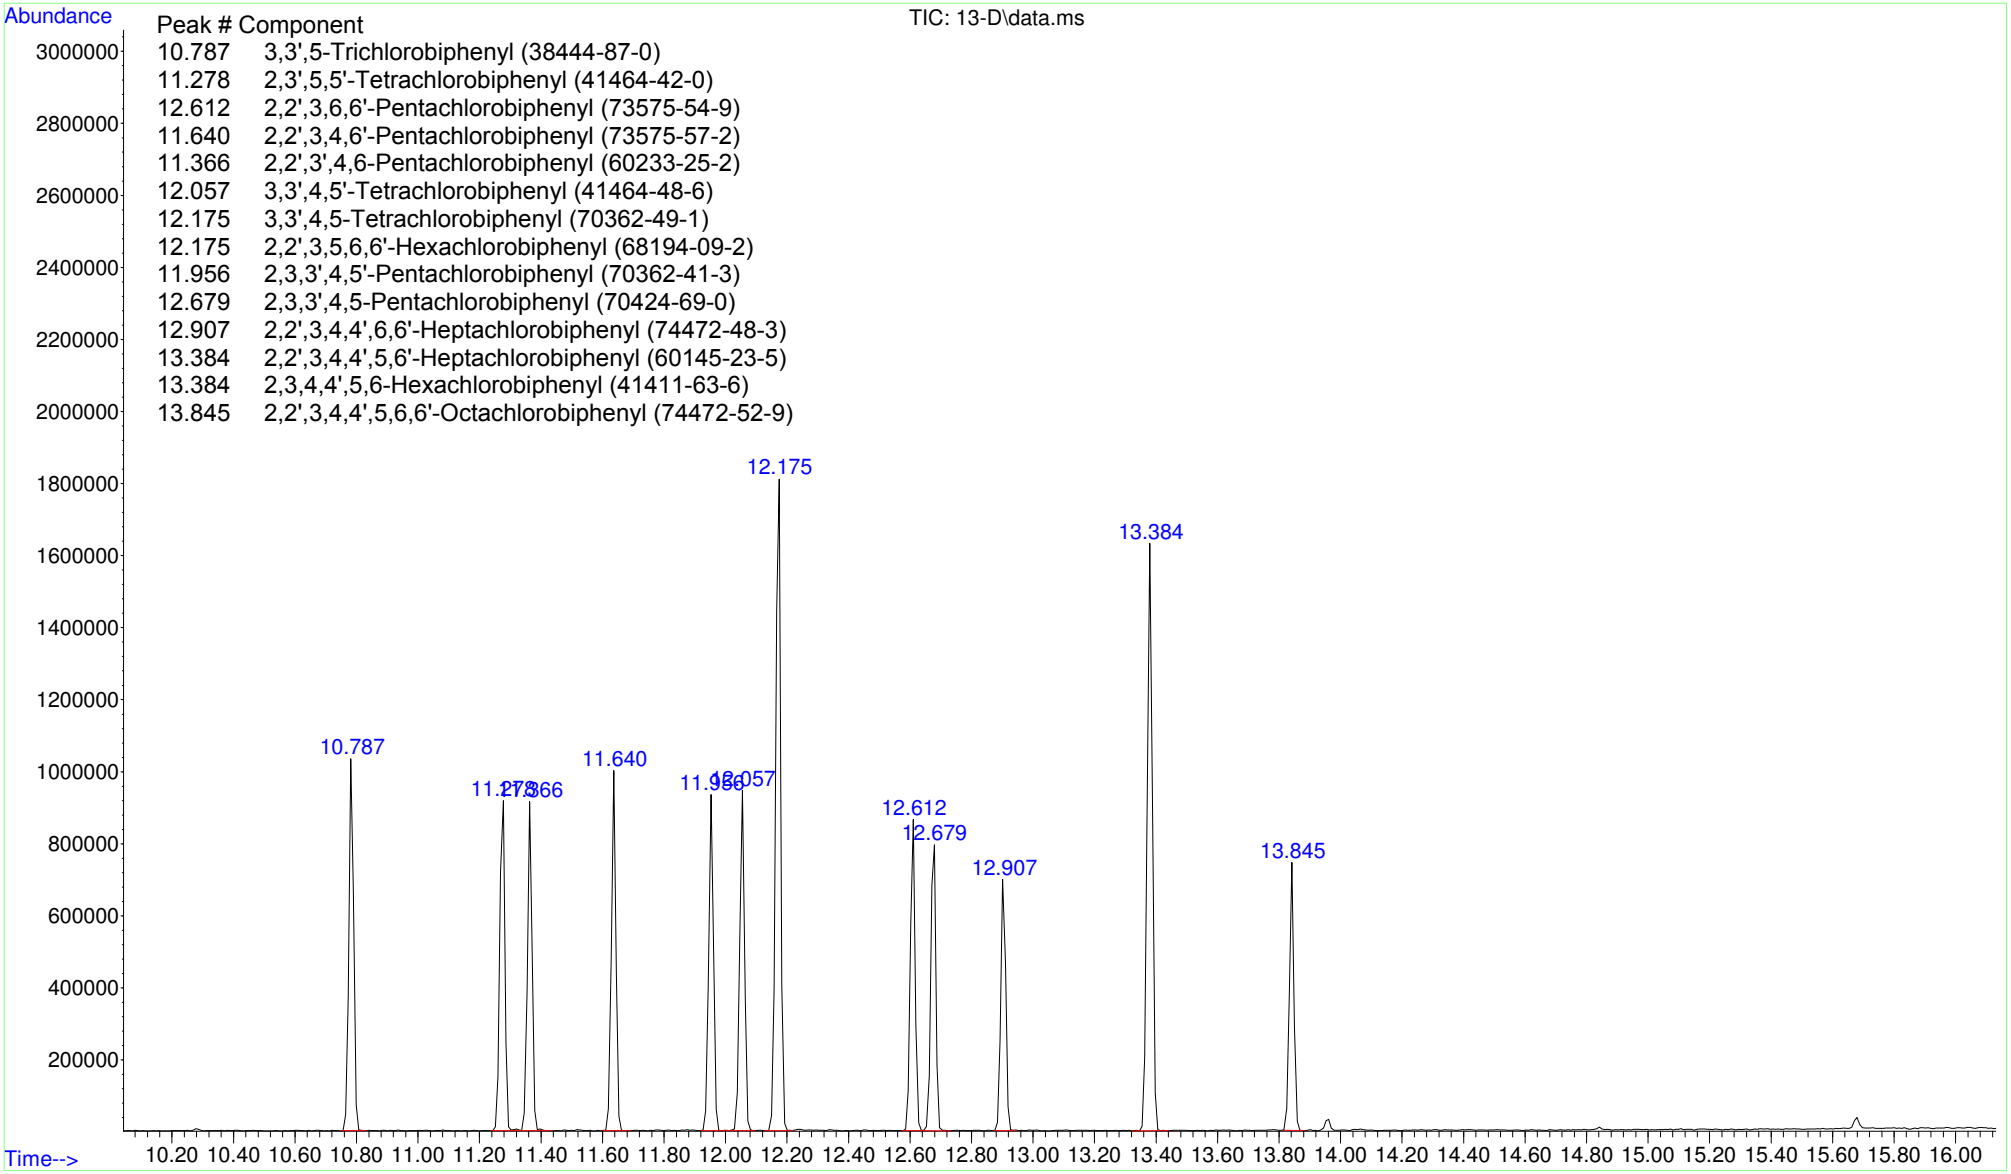
```
File        :D:\MassHunter\GCMS\1\data\10111801\13-
Operator    : K.D
Acquired    : 11 Oct 2018  12:26     using AcqMethod KERLA-2Split-2uL.M
Instrument :   5977B MSD
Sample Name: C-CS-07
Misc Info:   in Isooctane
Vial Number: 83
```