AccuStandard®
Leader in Analytical Reference Standards

File :D:\MassHunter\GCMS\1\data\08221901\09- D
Operator : KD
Acquired : 22 Aug 2019 10:00 using AcqMethod KERLA-2017.M
Instrument : 5977B MSD
Sample Name: DIN38407-18
Misc Info : in ACCN
Vial Number: 3
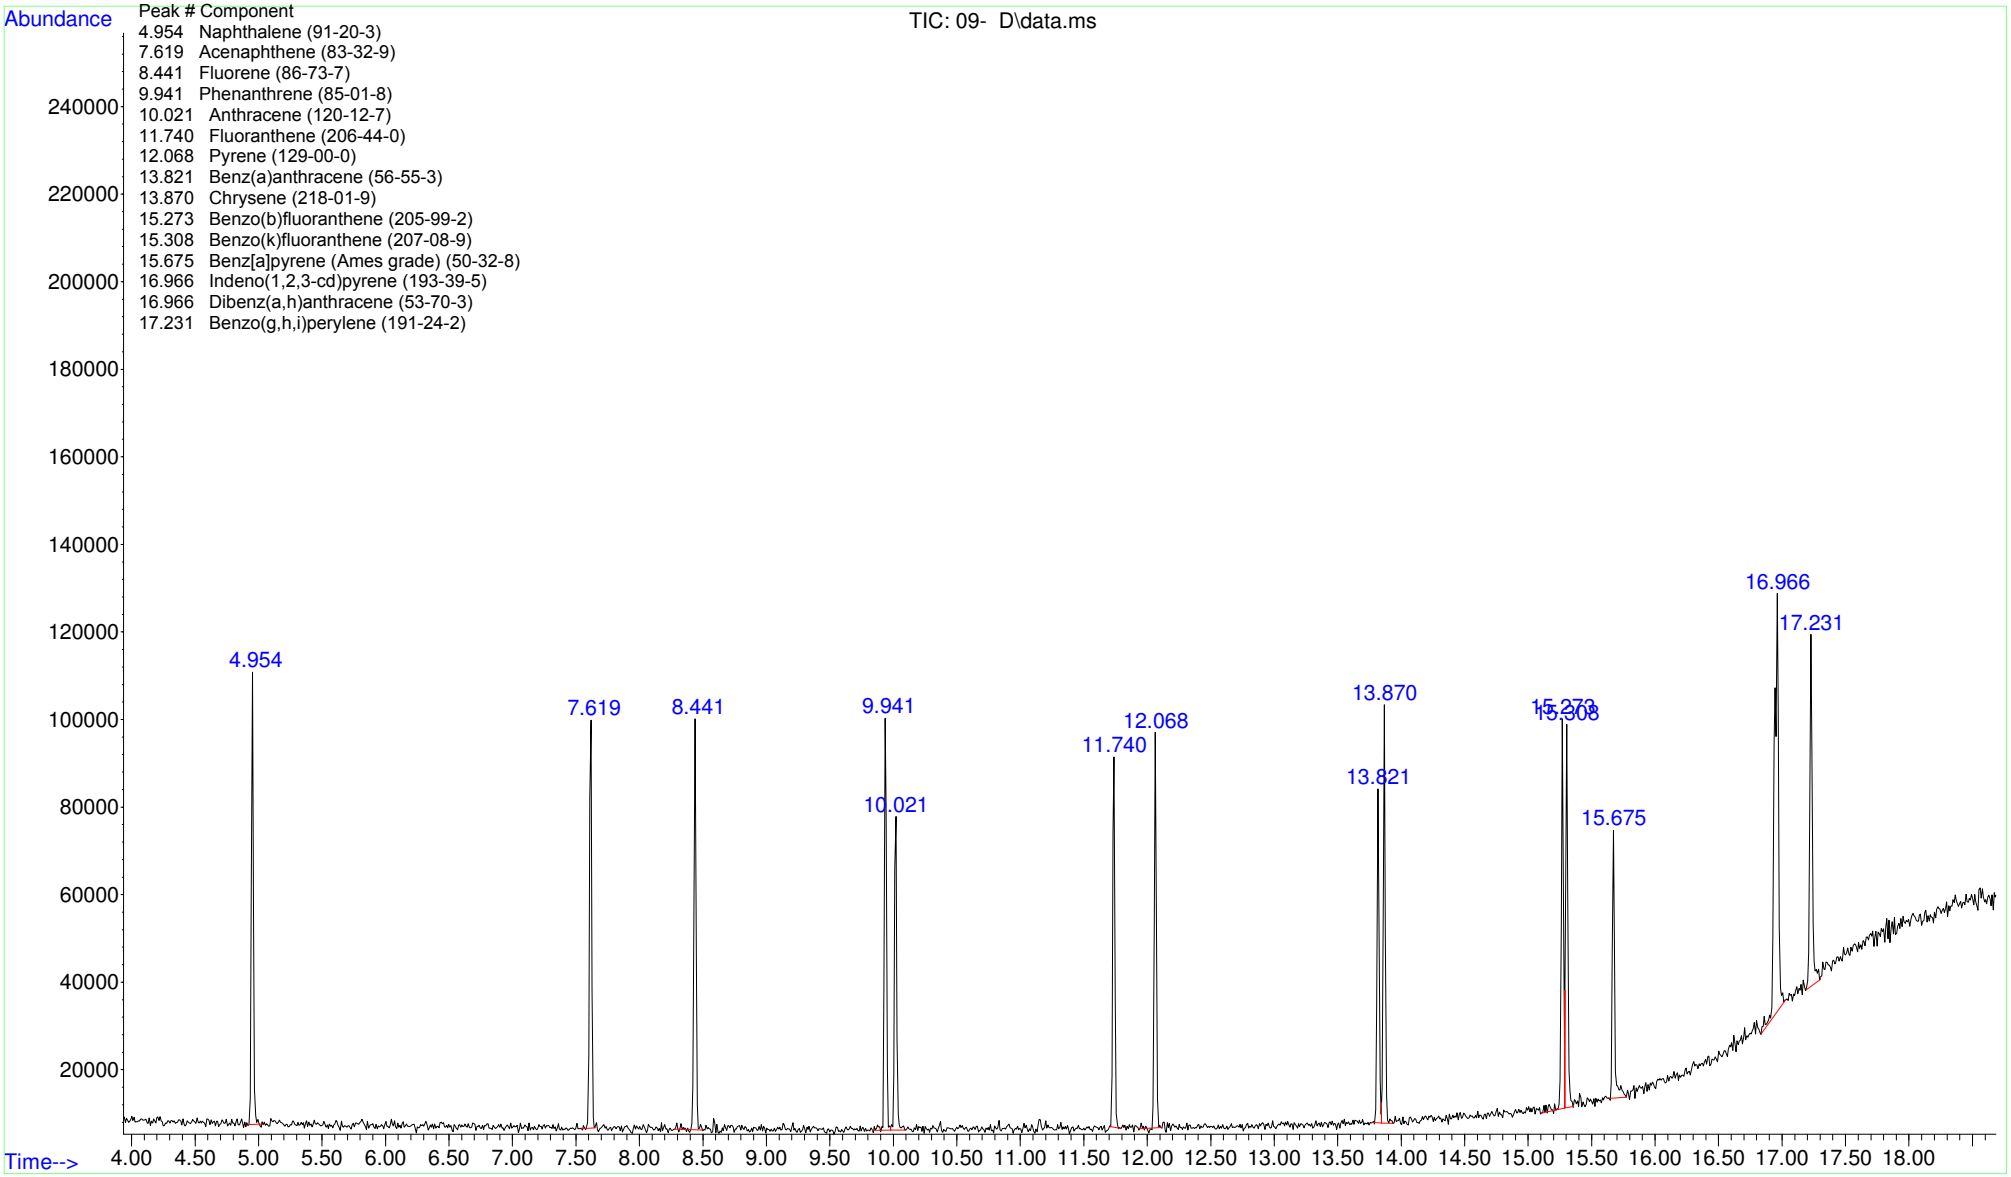
Column: DB-5, 30m, 0.25 ID, 0.25um
Oven Program: 100c, 1m, 30c/min to 320c, final 2min.
GC Parameters: Pulsed split 40psi 0.5m, 10psi constant flow
Split 20:1, 1ul inj.; GC/MS; INJ 250c.