


File : Q:\GCMS-06 Minimal\DATA\092721\30- KM.D
 Operator : Organic QC Lab
 Acquired : 27 Sep 2021 22:33 using AcqMethod CHICK_2019_2S_2uL.M
 Instrument : GCMS 6
 Sample Name: DINV38407-11-PST ()
 Misc Info : Pesticide Mix in AcCN
 Vial Number: 2



Column: DB-5MS UI, 30m x 0.25mm ID x 0.25µm
 Oven Program: 80°C, 17°C/min to 340°C (hold 8min)
 GC Parameters: Pulsed split 40psi 0.5min, 10psi constant flow
 Split 20:1, 1µl inj.; GC/MS; Injector 270°C

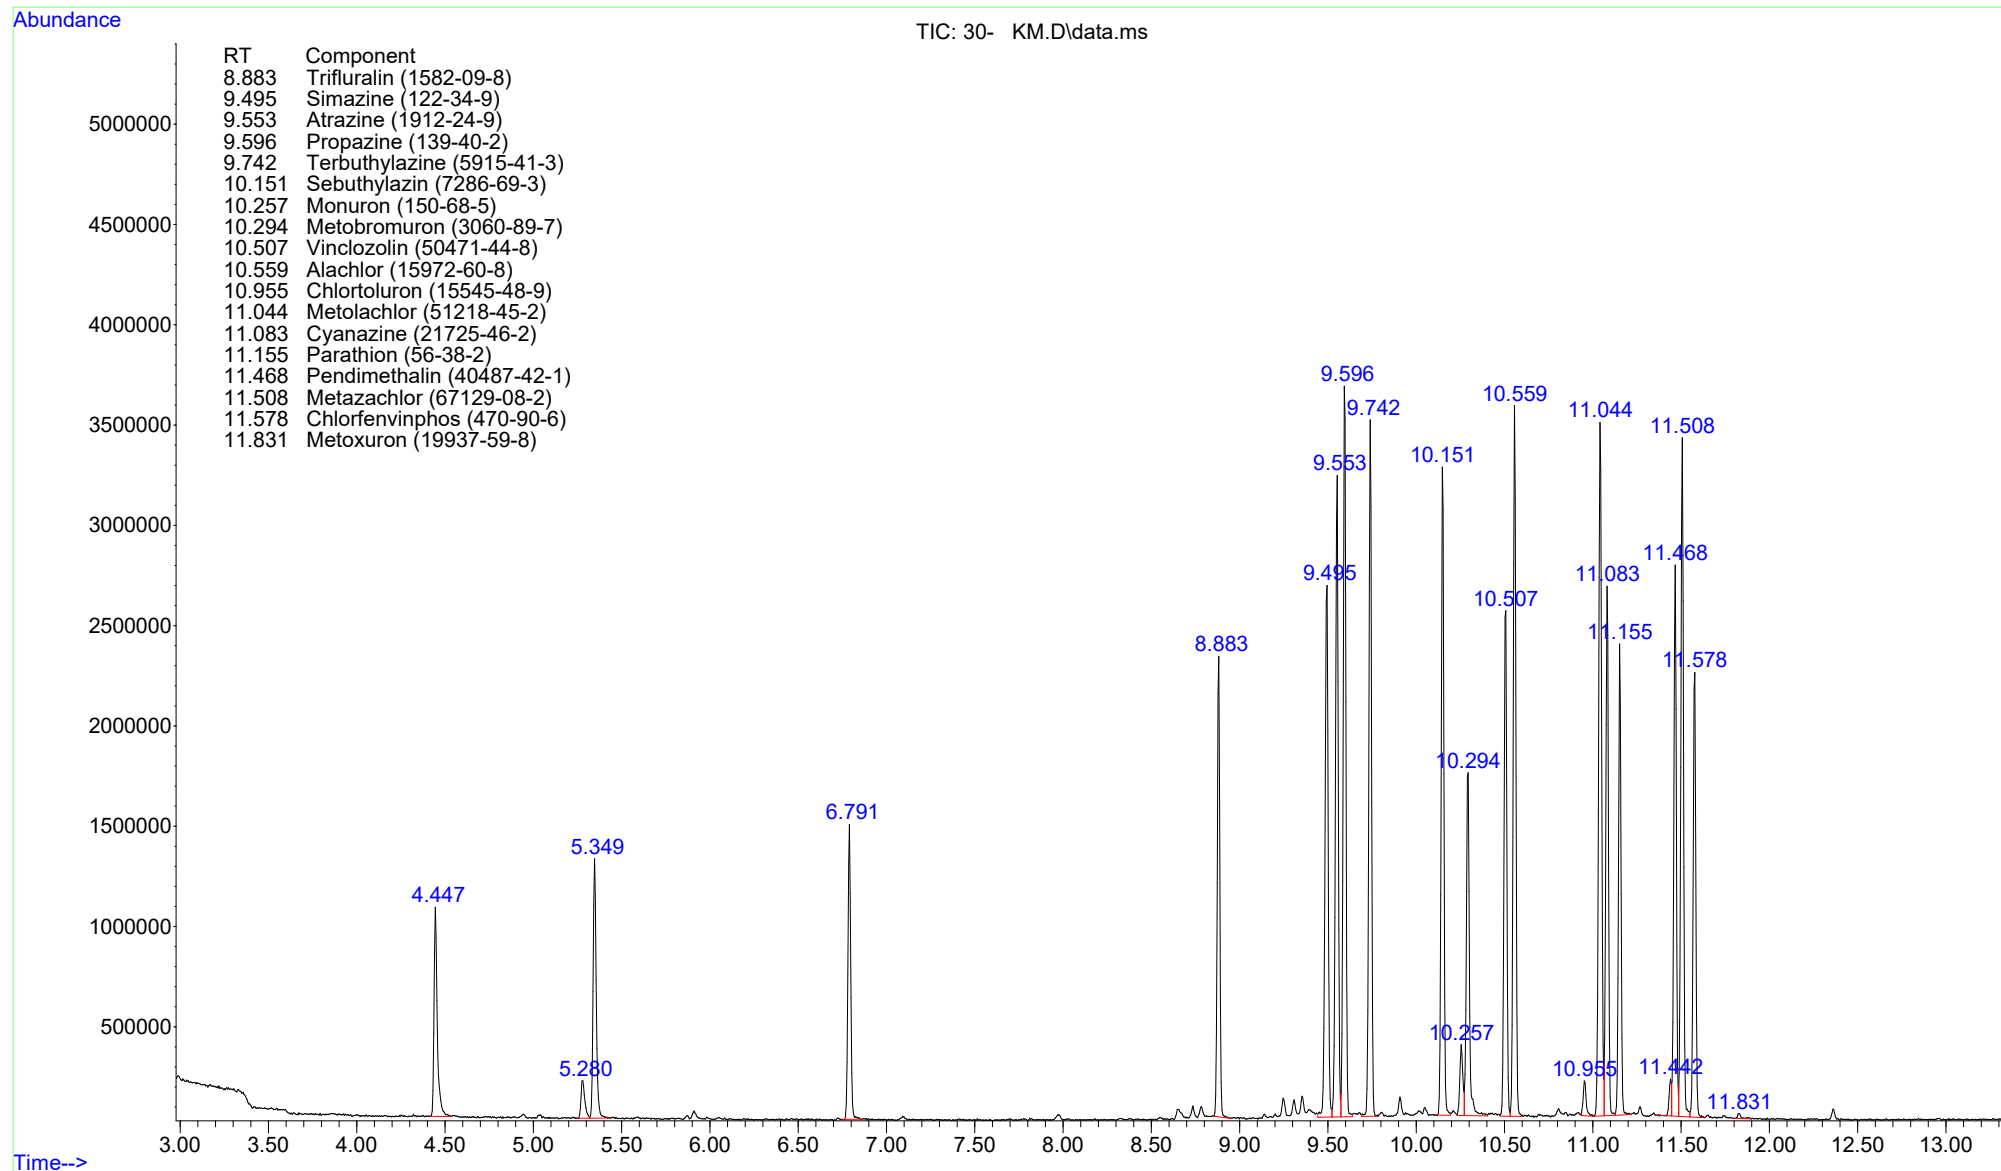

Cannot see on GC/MS - 2,4,5-T (93-76-5), 2,4-D (94-75-7), MCPA acid (94-74-6)