Print of window 38: Current Chromatogram(s)
Data File : C:\USERS\P...TION\1\DATA\06242001\06242001 2020-06-24 16-43-02\01-GA.D
Sample Name : DYE-017S-R1

==========

Acq. Operator : SYSTEM Seq. Line : 1
Sample Operator : SYSTEM
Acq. Instrument : LCMS-2 Location : P1-D-08
Injection Date : 6/24/2020 4:44:01 PM Inj : 1
Inj Volume : 1.000 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 2.000 µl
Acq. Method : C:\Users\Public\Documents\ChemStation\1\Data\06242001\06242001 2020-06-24 16-43-02 \Purity_195-315.M
Last changed : 5/8/2020 10:12:19 AM by SYSTEM
Analysis Method : C:\USERS\PUBLIC\DOCUMENTS\CHEMSTATION\1\METHODS\Purity_195-315.M
Last changed : 6/24/2020 12:11:23 PM by SYSTEM
(modified after loading)
Method Info : OPERATOR: Organic QC lab
General gradient method starting @100% water for 1 min @0.3 ml/min,the 100% Acetonitile in 13 min, 100% Acetonitrile until T=16 min. Column Zorbax Eclipse plus C-18, 2.1mmx50mm, 1.8 u particlue size. Agilent 1290 Infinity II LC/MS system , Agilent 6125 quadrupole MS detector.

Additional Info : Peak(s) manually integrated
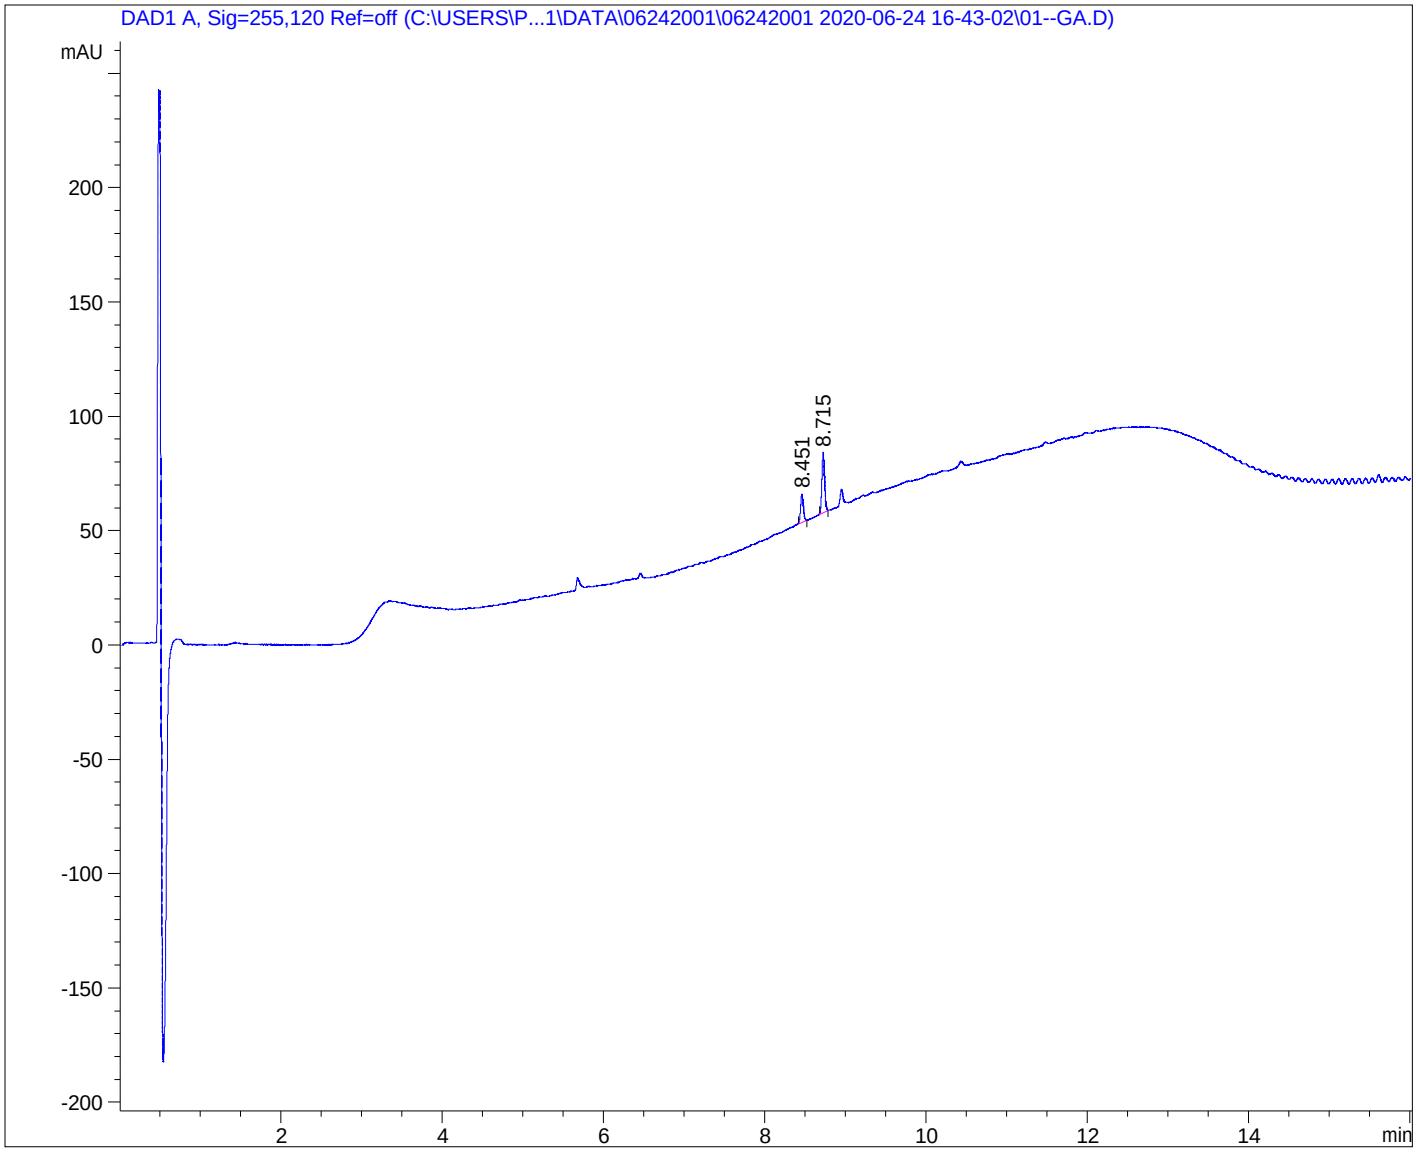
Current Chromatogram(s)