Print of window 38: Current Chromatogram(s)
Data File : D:\DATA\01162001\09- .D
Sample Name : HBDE-5006S-CN-0.2X

==========

Acq. Operator : SYSTEM Seq. Line : 1
Acq. Instrument : LCMS-1 Location : P1-B6
Injection Date : 1/16/2020 1:45:12 PM Inj : 1
Inj Volume : 1.000 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 10.000 µl
Method : C:\CHEM32\1\METHODS\Purity195_315.M
Last changed : 10/18/2019 4:18:14 PM by SYSTEM
Method Info : Operator: GA
Gradient Method Starting @ 100 % Water/0 % Acetonitrile to 0 % Water/100 % Acetonitrile in 13 min, then 3 min at 100/0, post-run time 2 min. Flow rate :0.3 ml/min, column Zorbax Eclipse Plus C-18, 2.1x50 mm, 1.8 micron particule size. Agilent 1290 Infinity II LC system, Agilent 6120 Quadrople MS Detector. No UV Reference.

Sample Info : 6'-Hydroxy-2,2',4,4',5-pentabromodiphenyl ether @10ug/mL in AcCN

Additional Info : Peak(s) manually integrated
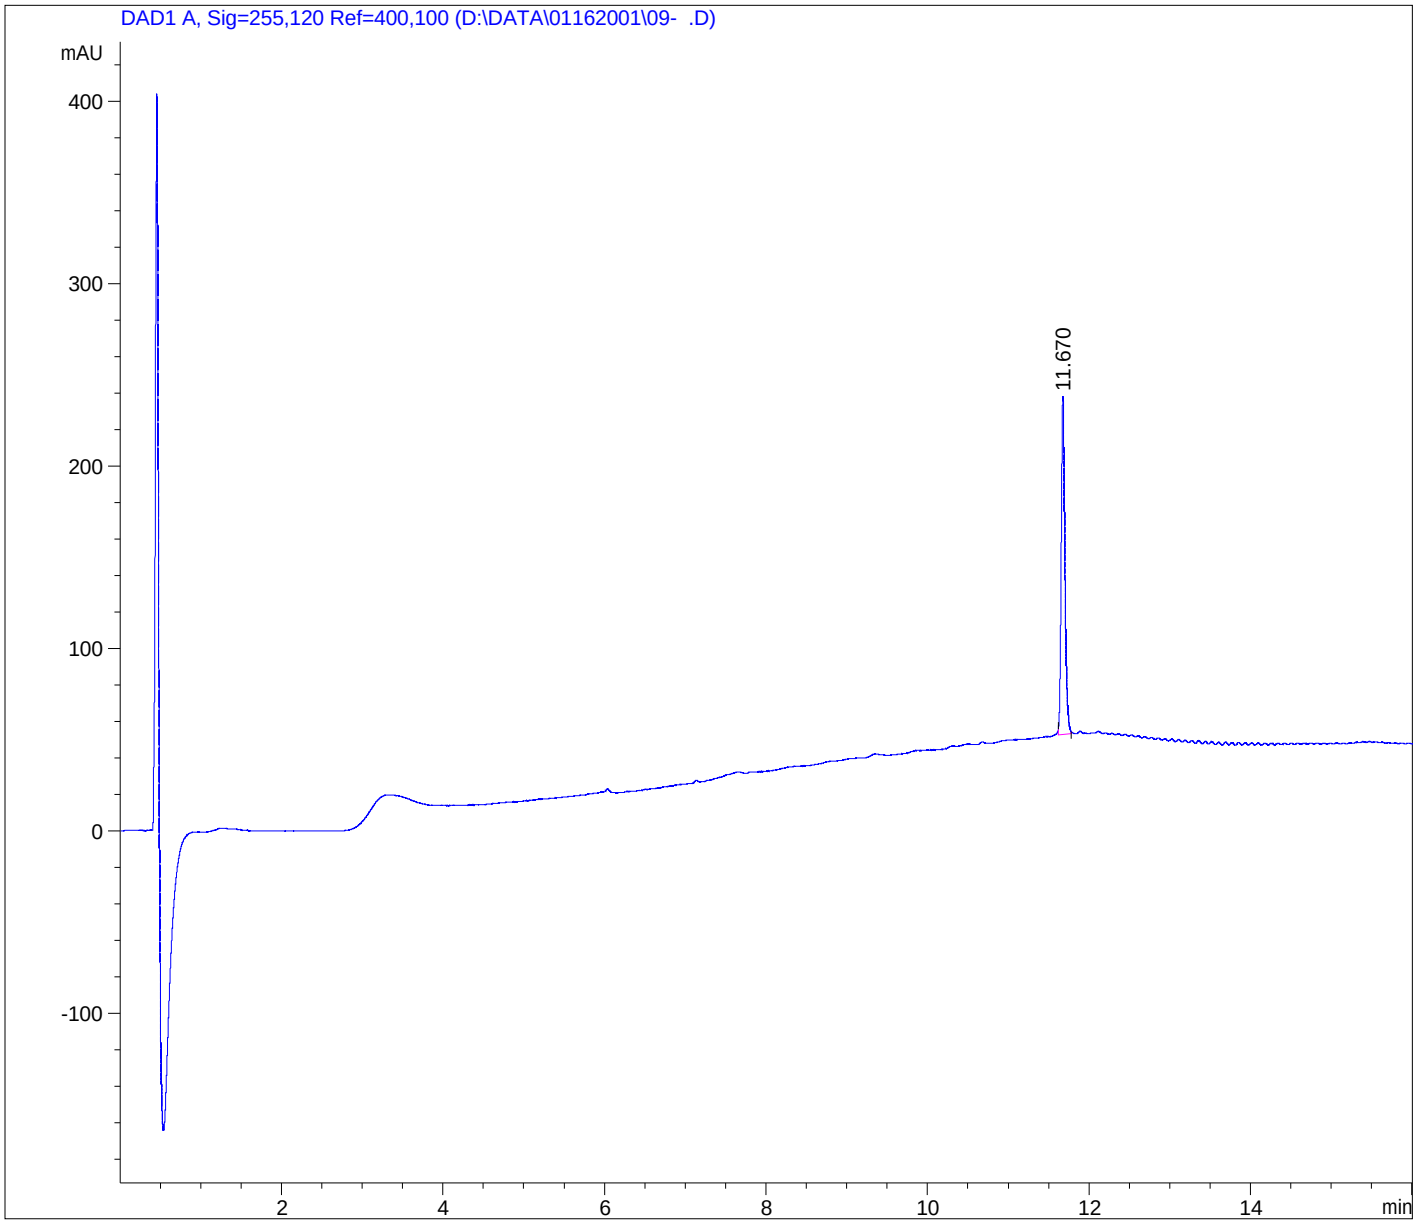
Current Chromatogram(s)