Print of window 38: Current Chromatogram(s)
Data File : C:\USERS\P...ON\1\DATA\06022201\06022201 2022-06-02 06-23-04\02- KD.D
Sample Name : M-547

==========

Acq. Operator : SYSTEM Seq. Line : 2
Sample Operator : SYSTEM
Acq. Instrument : LCMS-2 Location : P2-C9
Injection Date : 6/2/2022 6:30:03 AM Inj : 2
Inj Volume : 2.000 µl
Acq. Method : C:\Users\Public\Documents\ChemStation\1\Data\06022201\06022201 2022-06-02 06-23-04\Glyphosate.M
Last changed : 1/31/2020 3:41:23 PM by SYSTEM
Analysis Method : C:\USERS\PUBLIC\DOCUMENTS\CHEMSTATION\1\METHODS\Purity_195-315.M
Last changed : 5/16/2022 12:35:31 PM by SYSTEM
(modified after loading)
Method Info : OPERATOR: Organic QC lab
General gradient method starting @100% water for 1 min @0.3 ml/min,the 100% Acetonitile in 13 min, 100% Acetonitrile until T=16 min. Column Zorbax Eclipse plus C-18, 2.1mmx50mm, 1.8 u particlue size. Agilent 1290 Infinity II LC/MS system, Agilent 6125 quadrupole MS detector.
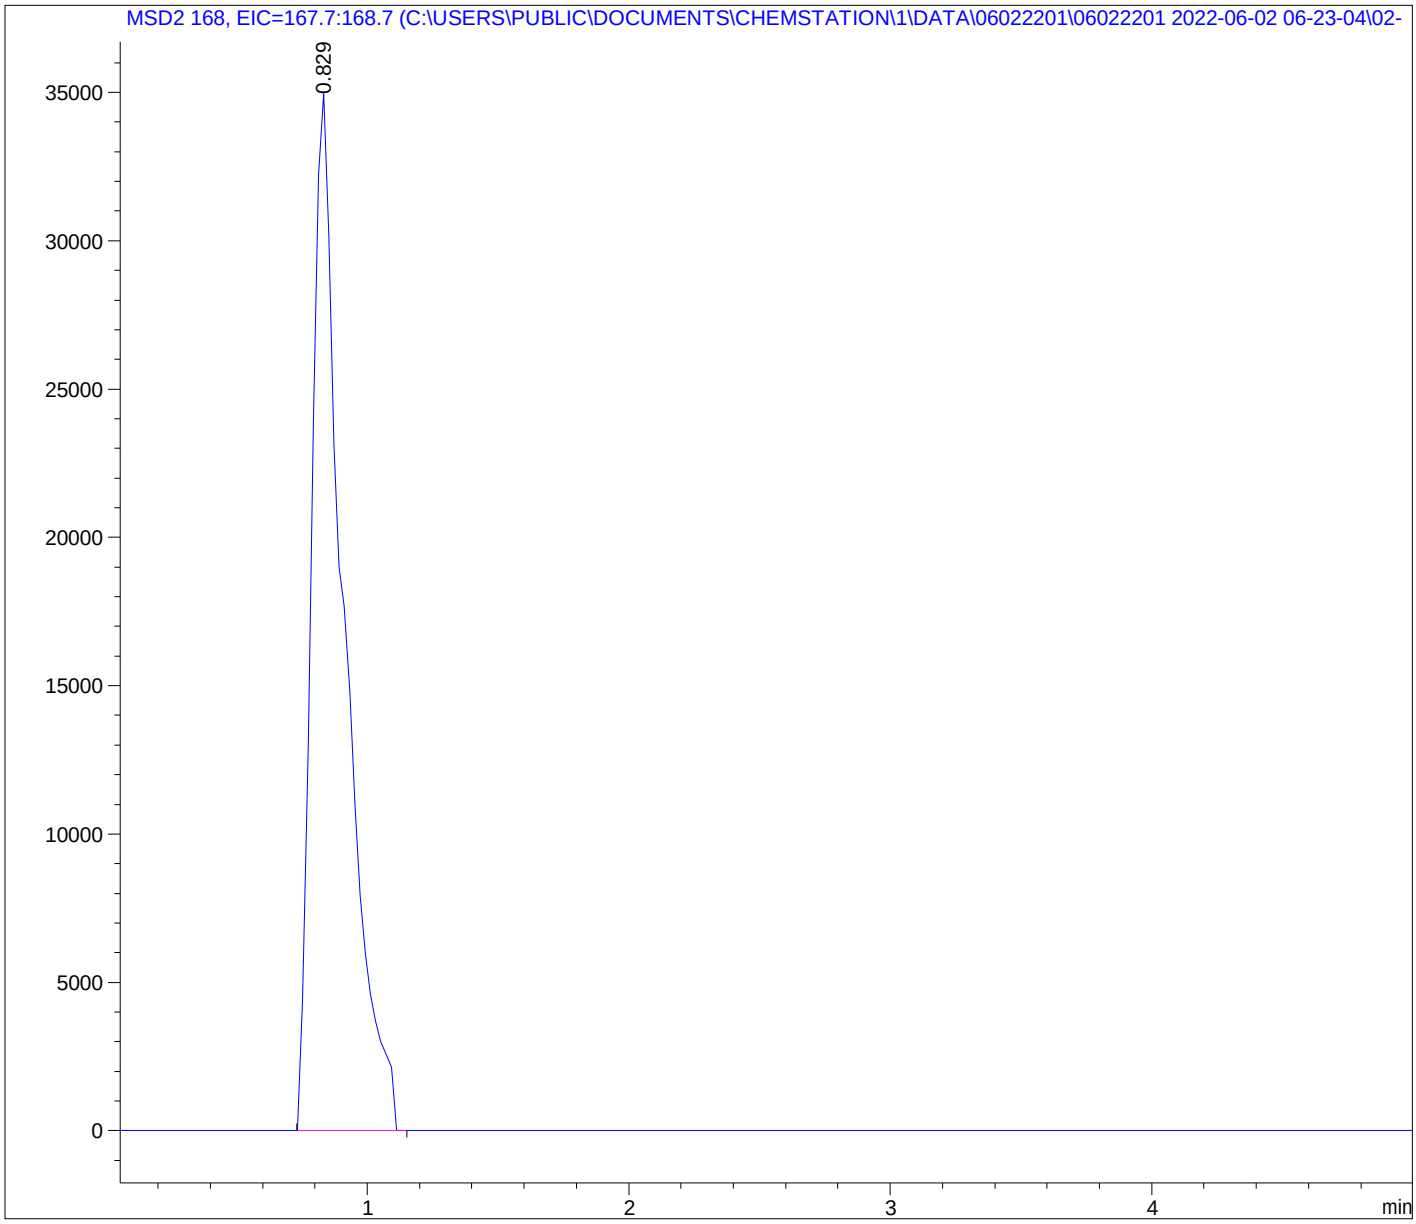
Current Chromatogram(s)