Print of window 38: Current Chromatogram(s)
Data File : D:\DATA\01142022\02- KM.D
Sample Name : M-632M

Acq. Operator : SYSTEM Seq. Line : 2
Acq. Instrument : LCMS-1 Location : P1-A7
Injection Date : 1/14/2022 2:59:54 PM Inj : 2
Inj Volume : 1.000 µl

Method : C:\CHEM32\1\METHODS\Purity195_315.M
Last changed : 11/5/2021 2:37:17 PM by SYSTEM
Method Info : Operator: Organic QC lab
Gradient Method Starting @ 100 % Water/0 % Acetonitrile to 0 % Water/100 % Acetonitrile in 13 min, then 3 min at 100/0, post-run time 2 min. Flow rate :0.3 ml/min, column Zorbax Eclipse Plus C-18, 2.1x50 mm, 1.8 micron particle size. Agilent 1290 Infinity II LC system, Agilent 6120 Quadrople MS Detector. No UV Reference.

Sample Info : RT: Carbamates & Urea Pesticides @ 100 ug/mL in AcCN

Additional Info : Peak(s) manually integrated

Current Chromatogram(s)

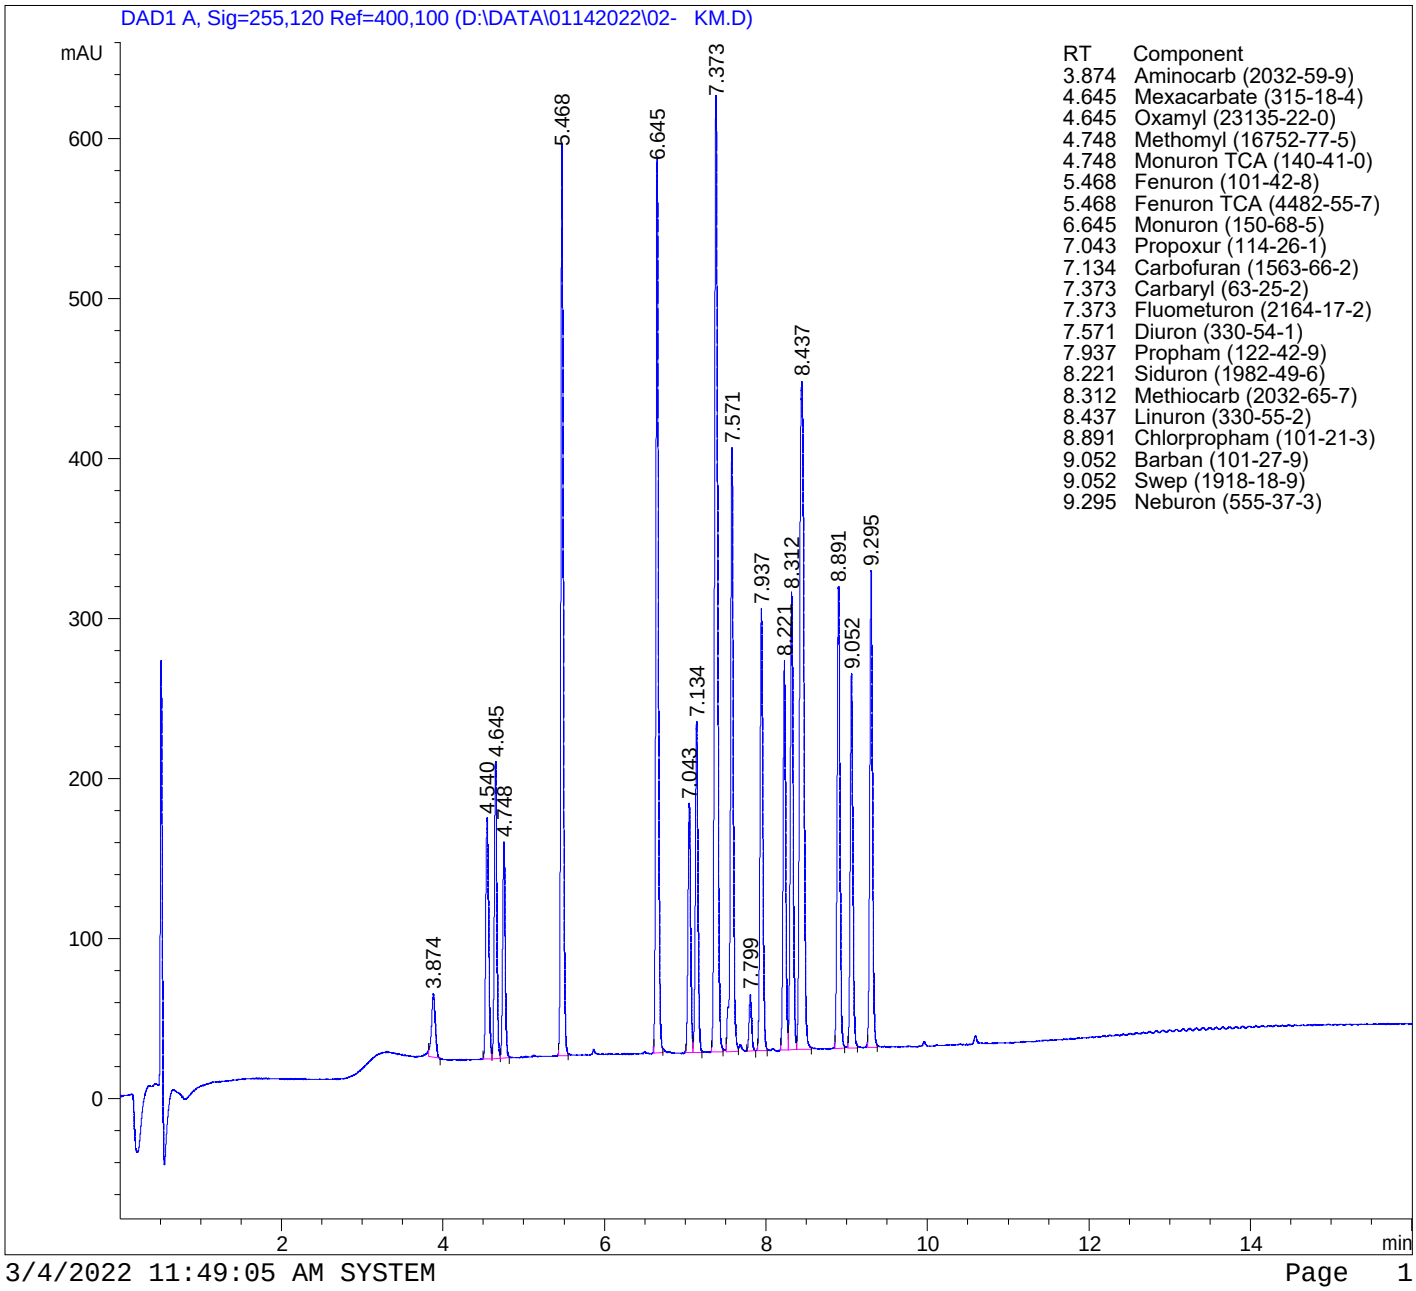

RT	Component
3.874	Aminocarb (2032-59-9)
4.645	Mexacarbate (315-18-4)
4.645	Oxamyl (23135-22-0)
4.748	Methomyl (16752-77-5)
4.748	Monuron TCA (140-41-0)
5.468	Fenuron (101-42-8)
5.468	Fenuron TCA (4482-55-7)
6.645	Monuron (150-68-5)
7.043	Propoxur (114-26-1)
7.134	Carbofuran (1563-66-2)
7.373	Carbaryl (63-25-2)
7.373	Fluometuron (2164-17-2)
7.571	Diuron (330-54-1)
7.937	Propham (122-42-9)
8.221	Siduron (1982-49-6)
8.312	Methiocarb (2032-65-7)
8.437	Linuron (330-55-2)
8.891	Chlorpropham (101-21-3)
9.052	Barban (101-27-9)
9.052	Swep (1918-18-9)
9.295	Neburon (555-37-3)