Print of window 38: Current Chromatogram(s)
Data File : D:\DATA\04092001\11 .D
Sample Name : M-8150-51-SS-WL-50ML

==========

Acq. Operator : SYSTEM Seq. Line : 9
Acq. Instrument : LCMS-1 Location : P1-F6
Injection Date : 4/9/2020 1:01:34 PM Inj : 1
Inj Volume : 1.000 µl

Acq. Method : C:\CHEM32\1\METHODS\Purity195_315.M
Last changed : 4/3/2020 3:07:25 PM by SYSTEM
Analysis Method : C:\CHEM32\1\METHODS\Purity195_315.M
Last changed : 4/7/2020 6:36:53 AM by SYSTEM
(modified after loading)

Method Info : Operator: GA
Gradient Method Starting @ 100 % Water/0 % Acetonitrile to 0 % Water/100 % Acetonitrile in 13 min, then 3 min at 100/0, post-run time 2 min. Flow rate :0.3 ml/min, column Zorbax Eclipse Plus C-18, 2.1x50 mm, 1.8 micron particule size. Agilent 1290 Infinity II LC system, Agilent 6120 Quadrople MS Detector. No UV Reference.

Sample Info : 2,4-Dichlorophenylacetic acid in Methanol

Additional Info : Peak(s) manually integrated
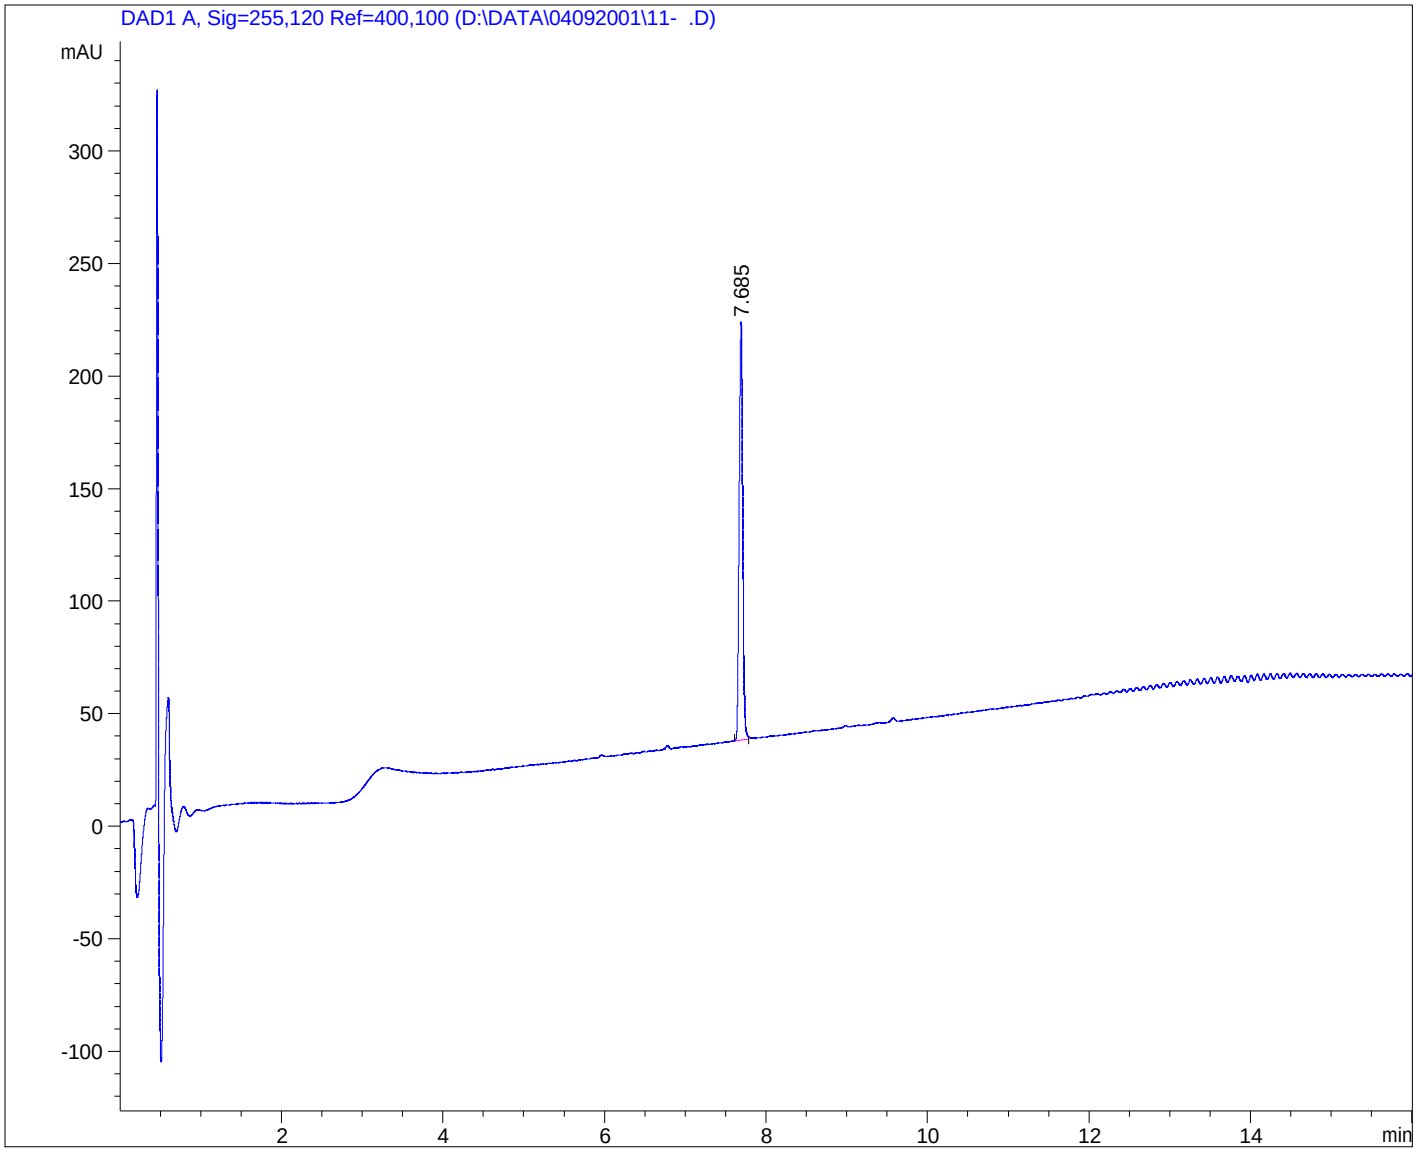
Current Chromatogram(s)