


File :Q:\GCMS-06 Minimal\DATA\091720\62- -DC.D
Operator : Organic QC Lab
Acquired : 17 Sep 2020 21:08 using AcqMethod CHICK_2019_S100.M
Instrument : GCMS 6
Sample Name: M-8270-16
Misc Info : in Acetone/DCM
Vial Number: 143



Column: DB-5MS UI, 30m x 0.25mm ID x 0.25µm
Oven Program: 80°C, 17°C/min to 340°C (hold 8min)
GC Parameters: Pulsed split 40psi 0.5min, 10psi constant flow
Split 20:1, 1µl inj.; GC/MS; Injector 270°C

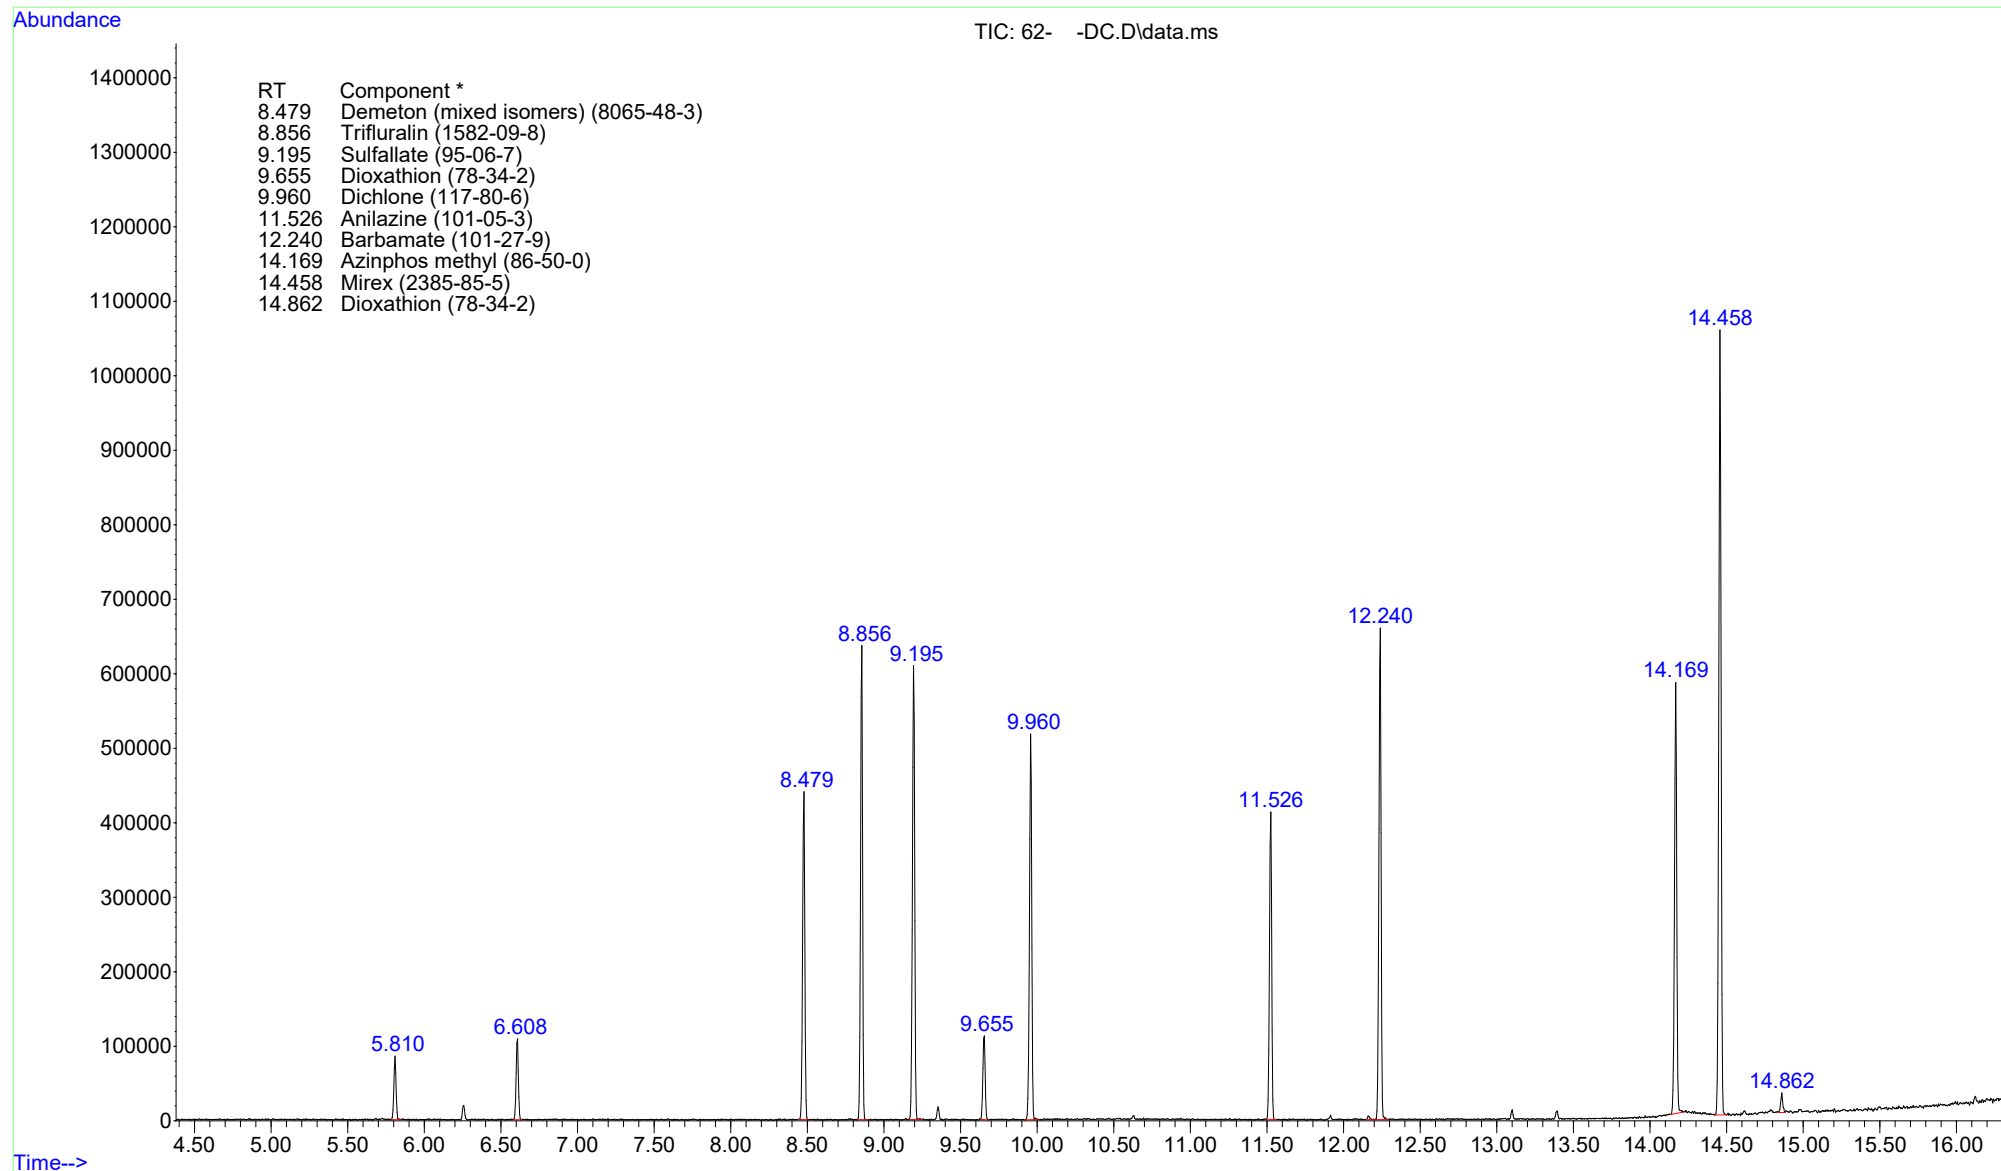

* Not seen by GC/MS - Sulfoxide (120-62-7)