Print of window 38: Current Chromatogram(s)
Data File : D:\DATA\10022001\01--GA.D
Sample Name : M-8315-R-DNPH-04

==========

Acq. Operator : SYSTEM Seq. Line : 1
Acq. Instrument : LCMS-1 Location : P2-A6
Injection Date : 10/2/2020 10:01:53 AM Inj : 1
Inj Volume : 1.000 µl

Acq. Method : C:\CHEM32\1\METHODS\DNPH.M
Last changed : 4/2/2018 12:14:16 PM by SYSTEM
Analysis Method : C:\CHEM32\1\METHODS\Purity195_315.M
Last changed : 10/1/2020 10:50:29 AM by SYSTEM
(modified after loading)
Method Info : Operator: Oraganic QC lab
Gradient Method Starting @ 100 % Water/0 % Acetonitrile to 0 % Water/100 % Acetonitrile in 13 min, then 3 min at 100/0, post-run time 2 min. Flow rate:0.3 ml /min, column Zorbax Eclipse Plus C-18, 2.1x50 mm, 1.8 micron particule size. Agilent 1290 Infinity II LC system, Agilent 6120 Quadrople MS Detector. No UV Reference.
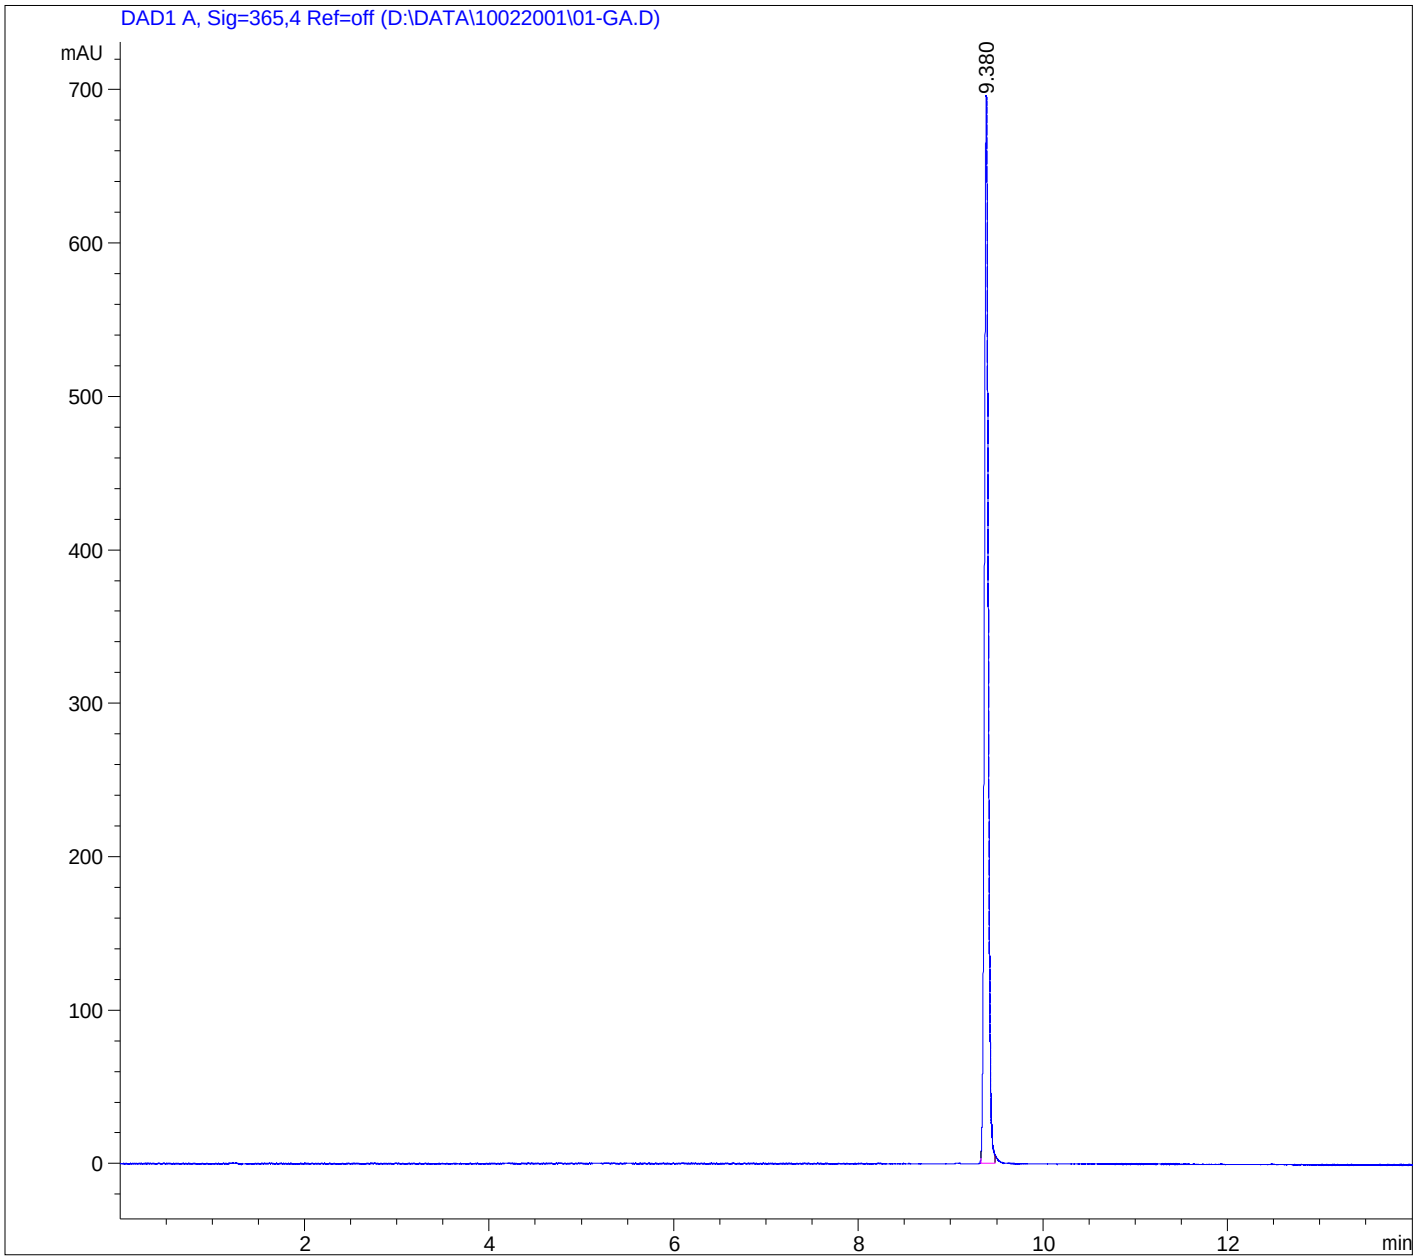
Current Chromatogram(s)