Print of window 38: Current Chromatogram(s)
Data File : C:\USERS\P...\1\DATA\01072201\01062201 2022-01-07 11-07-21\15 -KD.D
Sample Name : M-8315-R-DNPH-07

==========

Acq. Operator : SYSTEM Seq. Line : 15
Sample Operator : SYSTEM
Acq. Instrument : LCMS-2 Location : P2-E-01
Injection Date : 1/7/2022 3:32:29 PM Inj : 1
Inj Volume : 1.000 µl
Acq. Method : C:\Users\Public\Documents\ChemStation\1\Data\01072201\01062201 2022-01-07 11-07-21\Purity_195-315.M
Last changed : 4/29/2021 10:41:07 AM by SYSTEM
Analysis Method : C:\USERS\PUBLIC\DOCUMENTS\CHEMSTATION\1\METHODS\Purity_195-315.M
Last changed : 4/29/2021 10:41:07 AM by SYSTEM
Method Info : OPERATOR: Organic QC lab
General gradient method starting @100% water for 1 min @0.3 ml/min,the 100% Acetonitile in 13 min, 100% Acetonitrile until T=16 min. Column Zorbax Eclipse plus C-18, 2.1mmx50mm, 1.8 u particlue size. Agilent 1290 Infinity II LC/MS system, Agilent 6125 quadrupole MS detector.

Sample Info : Cyclohexanone-DNPH @ 100ug/mL in AcCN

Additional Info : Peak(s) manually integrated
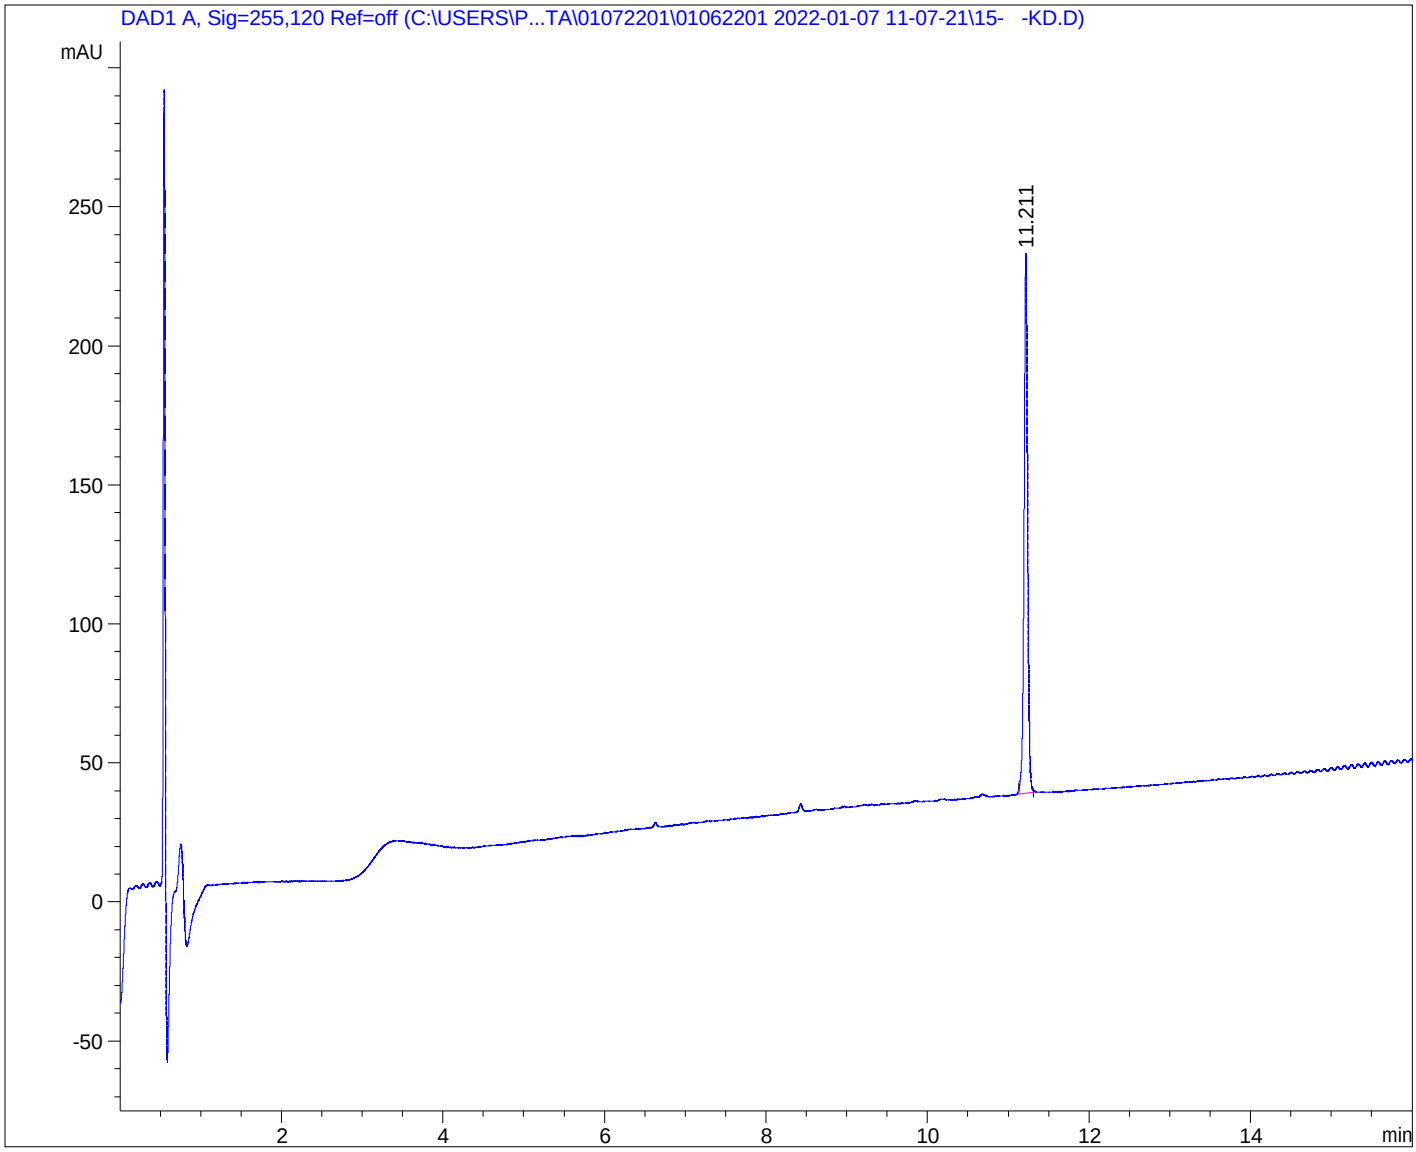
Current Chromatogram(s)