Print of window 38: Current Chromatogram(s)
Data File : D:\DATA\04122023\31- KM.D
Sample Name : M-8330-14-0.1X (223041179)

==========

Acq. Operator : SYSTEM Seq. Line : 31
Acq. Instrument : LCMS-1 Location : P1-D3
Injection Date : 4/12/2023 3:44:11 PM Inj : 1
Inj Volume : 1.000 µl

Acq. Method : C:\CHEM32\1\METHODS\Purity195_315.M
Last changed : 1/5/2023 12:01:53 PM by SYSTEM
Analysis Method : C:\CHEM32\1\METHODS\Purity195_315.M
Last changed : 4/12/2023 10:18:06 AM by SYSTEM
(modified after loading)
Method Info : Operator: Organic QC lab
Gradient Method Starting @ 100 % Water/0 % Acetonitrile to 0 % Water/100 % Acetonitrile in 13 min, then 3 min at 100/0, post-run time 2 min. Flow rate :0.3 ml/min, column Zorbax Eclipse Plus C-18, 2.1x50 mm, 1.8 micron particle size. Agilent 1290 Infinity II LC system, Agilent 6120 Quadrople MS Detector. No UV Reference.

Sample Info : 4-Amino-2,6-dinitrotoluene in 50:50 AcCN/MeOH

Additional Info : Peak(s) manually integrated
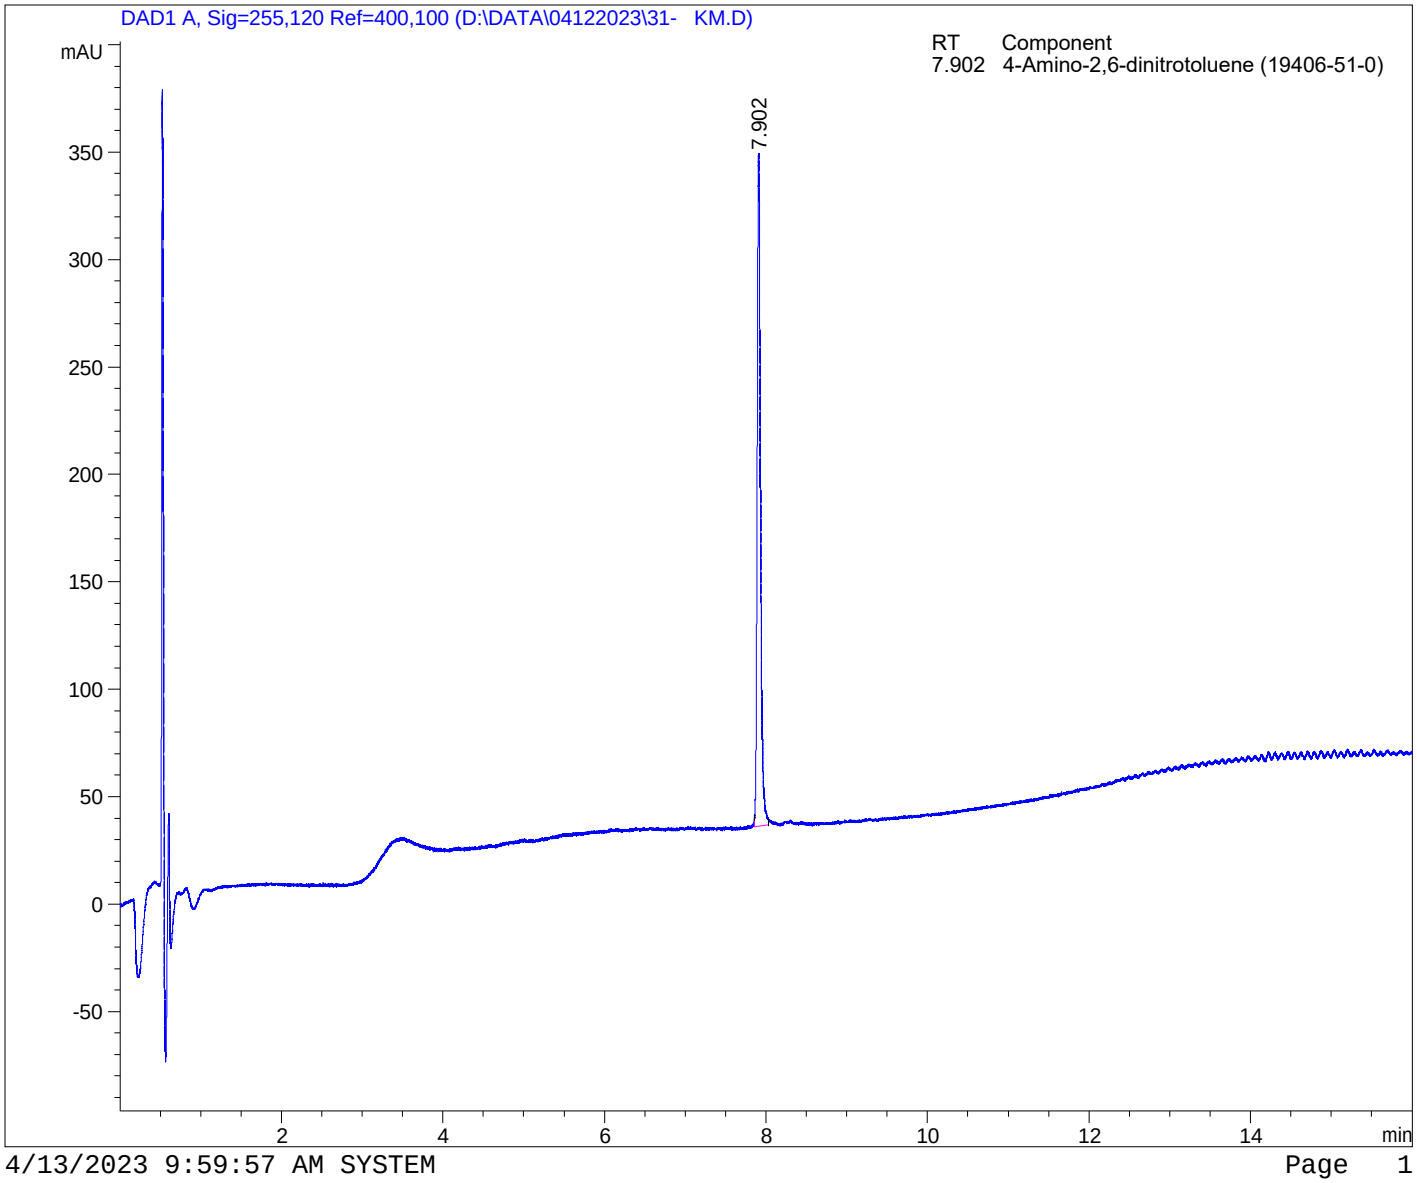
Current Chromatogram(s)