Print of window 38: Current Chromatogram(s)
Data File : D:\DATA\04052021\02-KD.D
Sample Name : M-8330-ADD-49

AccuStandard®
Leader in Analytical Reference Standards

Acq. Operator	: SYSTEM	Seq. Line	: 2
Acq. Instrument	: LCMS-1	Location	: P1-A1
Injection Date	: 4/5/2021 9:19:23 AM	Inj	: 2
		Inj Volume	: 1.000 µl

Acq. Method : C:\CHEM32\1\METHODS\Purity195_315.M
Last changed : 5/8/2020 11:20:44 AM by SYSTEM
Analysis Method : C:\CHEM32\1\METHODS\Purity195_315.M
Last changed : 3/31/2021 3:04:04 PM by SYSTEM
(modified after loading)
Method Info : Operator: Oraganic QC lab
Gradient Method Starting @ 100 % Water/0 % Acetonitrile to 0 % Water/100 % Acetonitrile in 13 min, then 3 min at 100/0, post-run time 2 min. Flow rate:0.3 ml /min, column Zorbax Eclipse Plus C-18, 2.1x50 mm, 1.8 micron particule size. Agilent 1290 Infinity II LC system, Agilent 6120 Quadrople MS Detector. No UV Reference.

Additional Info : Peak(s) manually integrated
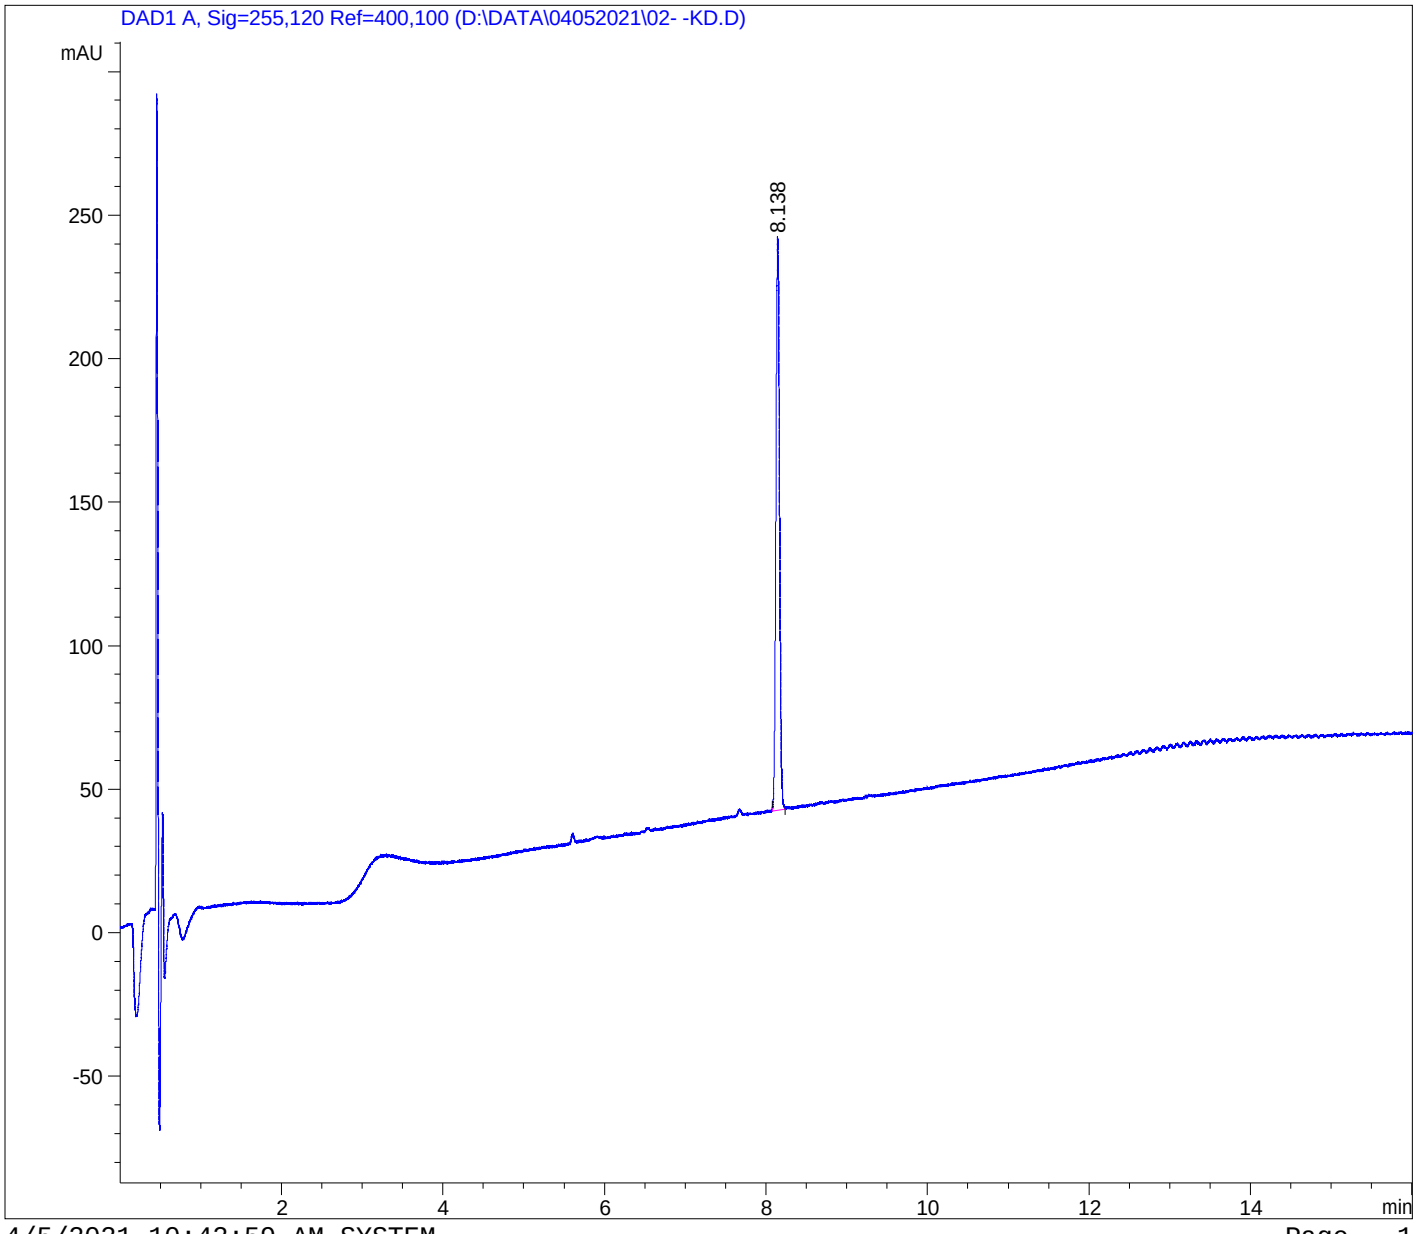
Current Chromatogram(s)