


File :Q:\GCMS-04\DATA\030419\09-D  
Operator : RFXM  
Acquired : 4 Mar 19 7:48 pm using AcqMethod VOC-SCAN 24 DECKER.M  
Instrument : GCMS4  
Sample Name: M-GRO-CAL-IS-02-R1  
Misc Info :  
Vial Number: 40



Column: DB-624 UI, 30m x 0.25mm ID x 1.4µm  
Oven Program: 35°C (hold 5min), 11°C/min to 60°C, 22°C/min to 230°C (hold 4min)  
GC Parameters: Split 100:1, 1µl inj.; GC/MS; Injector temp 240°C

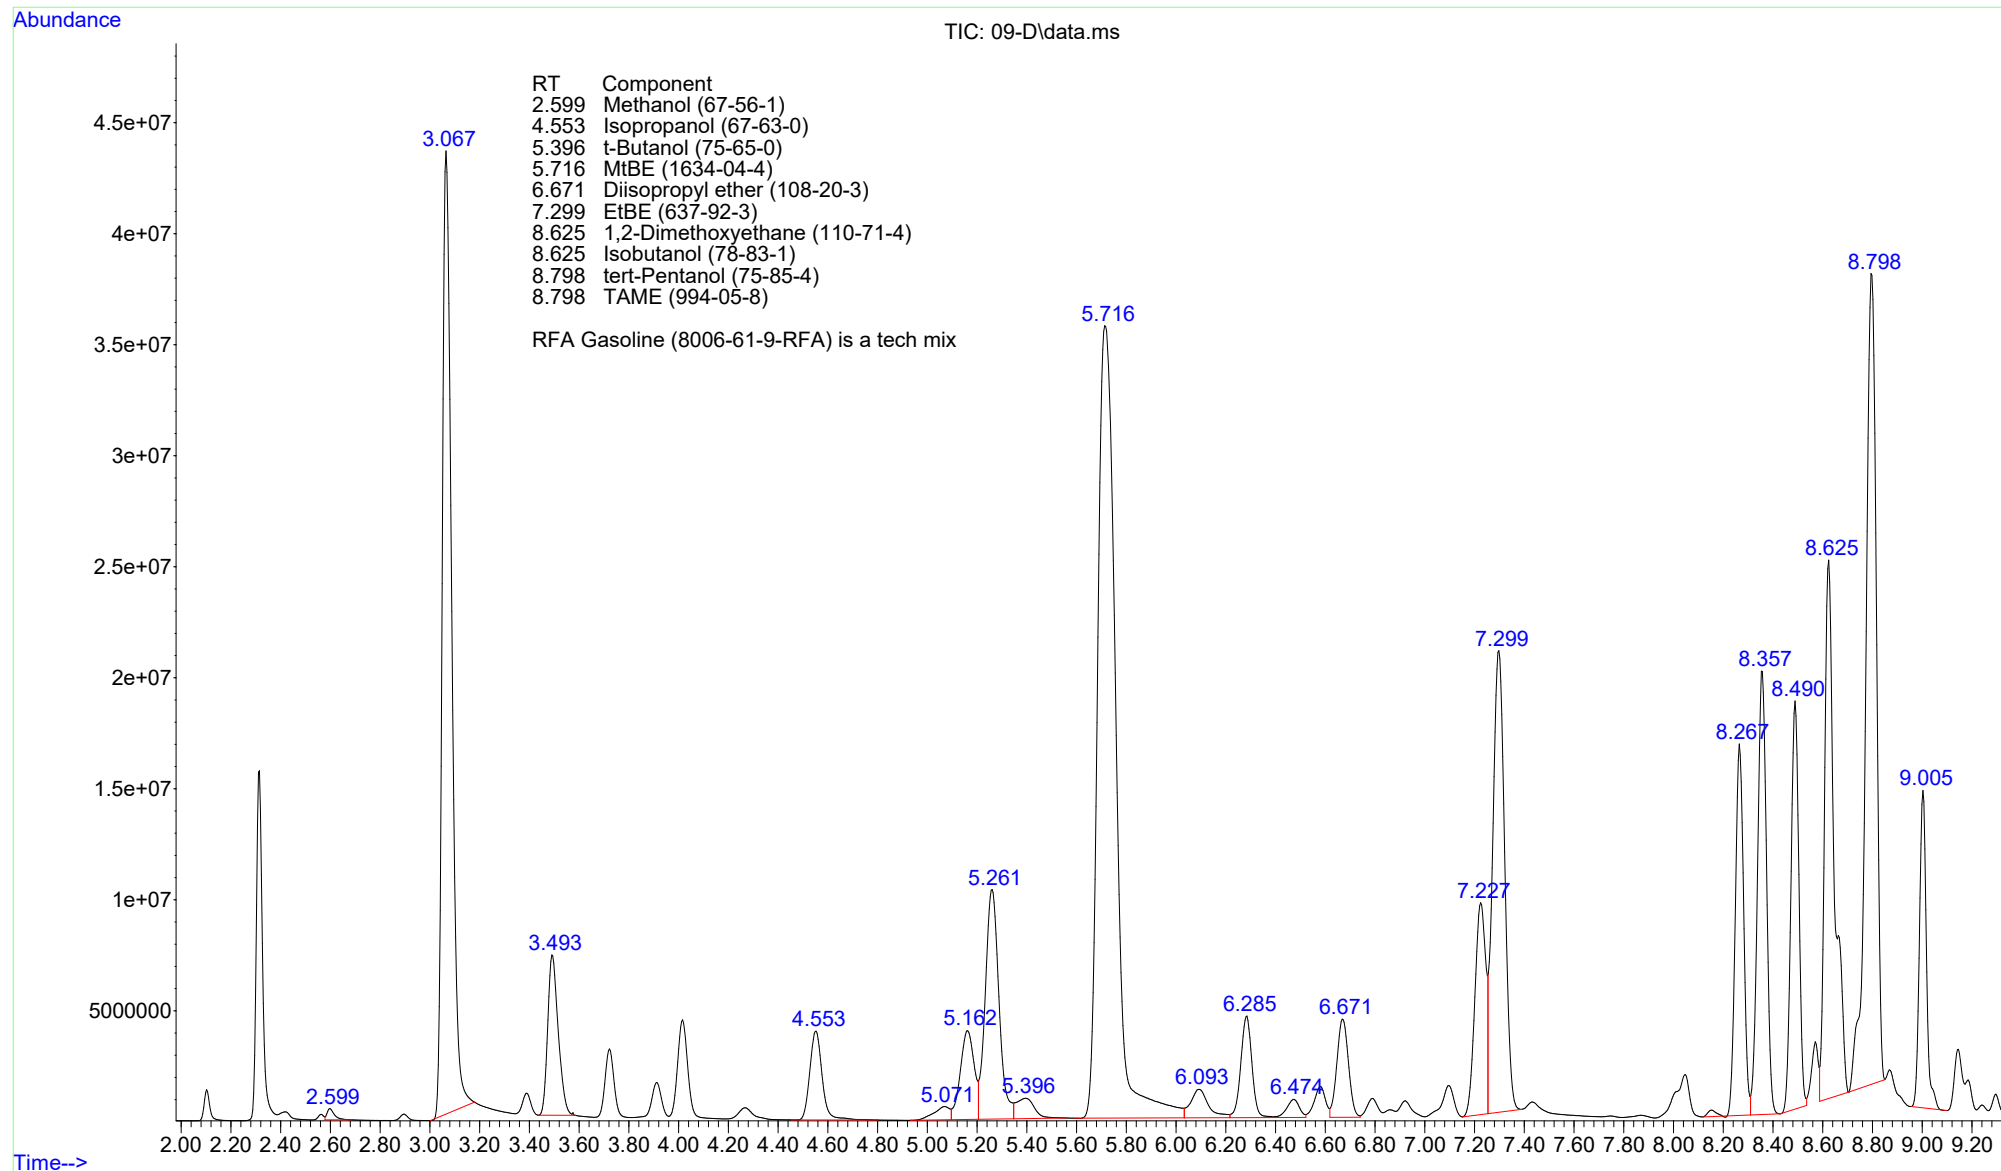

Not in mix - Ethanol (64-17-5), Propanol (71-23-8), sec-Butanol (78-92-2), 1-Butanol (71-36-3)