


File :Q:\GCMS-04\DATA\030419\13-.D
Operator : RFXM
Acquired : 4 Mar 2019 21:38 using AcqMethod VOC-SCAN 24 DECKER.M
Instrument : GCMS4
Sample Name: M-GRO-CAL-IS-03-R1
Misc Info :
Vial Number: 42



Column: DB-624 UI, 30m x 0.25mm ID x 1.4µm
Oven Program: 35°C (hold 5min), 11°C/min to 60°C, 22°C/min to 230°C (hold 4min)
GC Parameters: Split 100:1, 1µl inj.; GC/MS; Injector temp 240°C

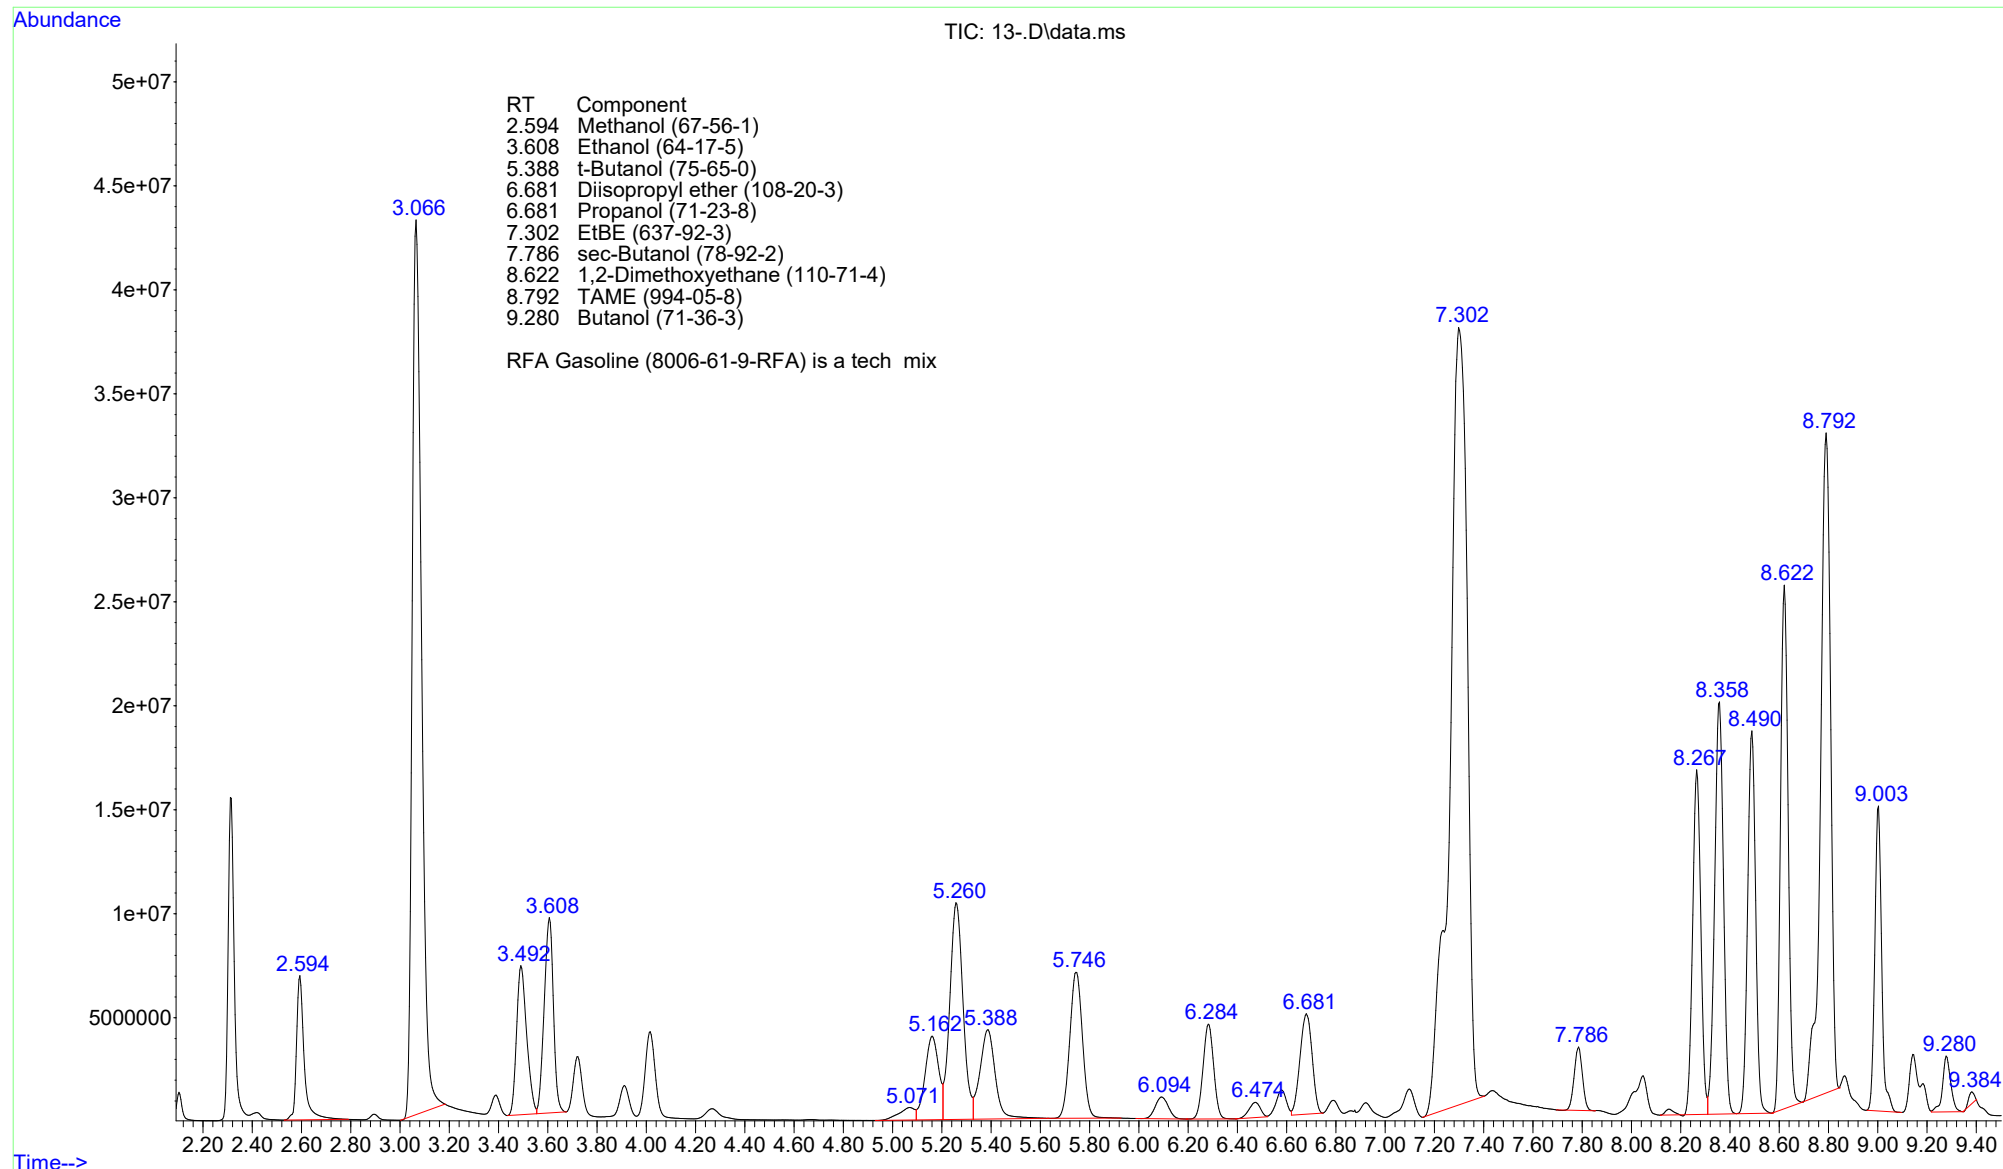

Not in mix - Isopropanol (67-63-0), MtBE (1634-04-4), Isobutanol (78-83-1), tert-Pentanol (75-85-4)