Print of window 38: Current Chromatogram(s)
Data File : C:\CHEM32\1\DATA\07231804\07231804 2018-07-23 12-25-06\Sample Name : P-952S-10X Chlorantraniprole

AccuStandard®

| | | | |
|---|---|---|---|
| Acq. Operator | : SYSTEM | Seq. Line : | 1 |
| Acq. Instrument | : LCMS-1 | Location : | P2-E3 |
| Injection Date | : 7/23/2018 12:25:51 PM | Inj : | 1 |
| | | Inj Volume : | 1.000 µl |

Acq. Method : C:\Chem32\1\Data\07231804\07231804 2018-07-23 12-25-06\PURITY195_315.M
Last changed : 7/23/2018 12:25:06 PM by SYSTEM
Analysis Method : C:\Chem32\1\Data\07231802\07231802 2018-07-23 11-29-02\Purity195_315.M (Sequence Method)
Last changed : 7/23/2018 11:29:02 AM by SYSTEM
Method Info : Operator: GA
Gradient Method Starting @ 100 % Water/0 % Acetonitrile to 0 % Water /100 % Acetonitrile in 13 min, then 3 min at 100/0, post-run time 2 min . Flow rate:0.3 ml/min, column Zorbax Eclipse Plus C-18, 2.1x50 mm, 1.8 micron particule size. Agilent 1290 Infinity II LC system, Agilent 6120 Quadrople MS Detector. No UV Reference.

Sample Info : Chlorantraniprole

Additional Info : Peak(s) manually integrated
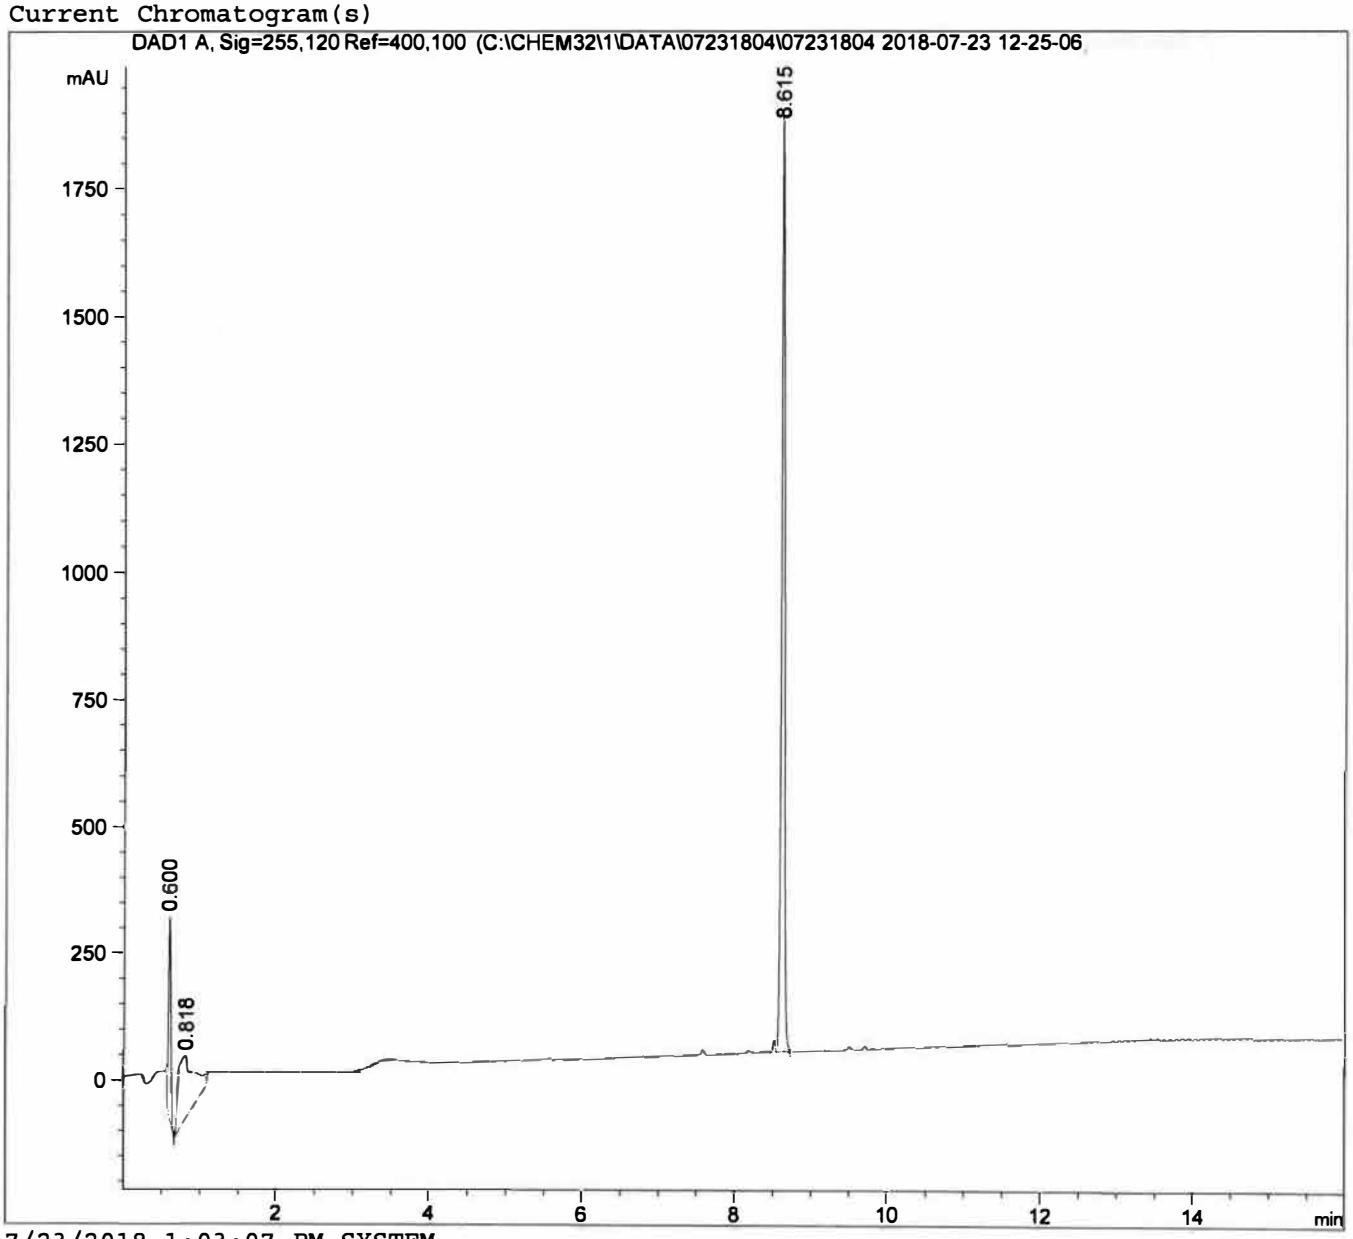
Current Chromatogram(s)