Print of window 38: Current Chromatogram(s)
Data File :D:\DATA\06061801\06061801 2018-06-06 10-34-26\08-
Sample Name : P-966S-CN-10X

==========

AccuStandard®
Leader in Analytical Reference Standards

Novaluron

Acq. Operator	: SYSTEM	Seq. Line :	6
Acq. Instrument	: LCMS-1	Location :	P1-C9
Injection Date	: 6/6/2018 12:27:48 PM	Inj :	1
		Inj Volume :	1.000 µl

Acq. Method : D:\DATA\06061801\06061801 2018-06-06 10-34-26\Purity195_315.M
Last changed : 6/6/2018 10:34:27 AM by SYSTEM
Analysis Method : C:\Chem32\1\Methods\Purity195_315.M
Last changed : 6/6/2017 9:45:25 AM by SYSTEM
Method Info : Operator: GA
Gradient Method Starting @ 100 % Water/0 % Acetonitrile to 0 % Water /100 % Acetonitrile in 13 min, then 3 min at 100/0, post-run time 2 min . Flow rate:0.3 ml/min, column Zorbax Eclipse Plus C-18, 2.1x50 mm, 1.8 micron particule size. Agilent 1290 Infinity II LC system, Agilent 6120 Quadrople MS Detector. No UV Reference.

Additional Info : Peak(s) manually integrated
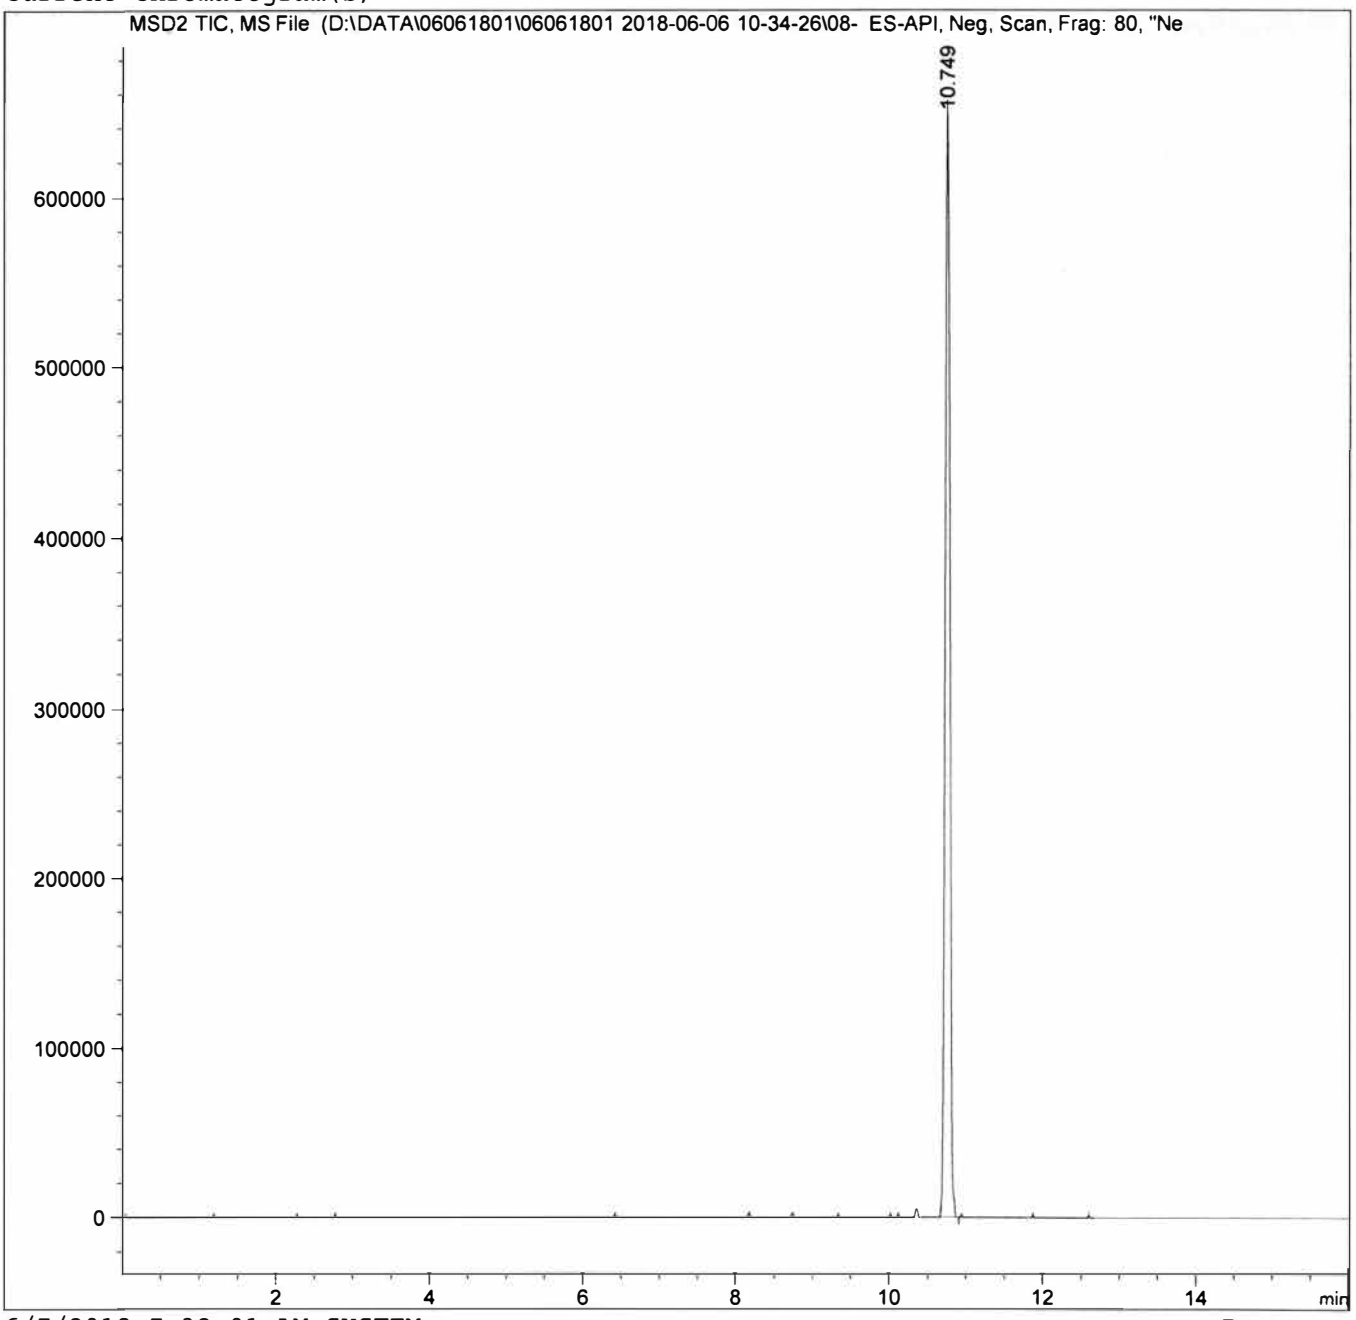
Current Chromatogram(s)