

Sample Name: PFOA-006S





```

=====
Acq. Operator   : SYSTEM                               Seq. Line :
Sample Operator : SYSTEM                               Location  : P1-F-06
Acq. Instrument : LCMS-2                               Inj       : 1
Injection Date  : 4/13/2023 12:07:30 PM              Inj Volume: 2.000 µl
                                                    Actual Inj Volume: 0.500 µl
Different Inj Volume from Sample Entry!
Acq. Method     : C:\Users\Public\Documents\ChemStation\1\Data\041323\032123101 2023-04-13 07-23-33\PFAA.M
Last changed    : 1/26/2021 10:30:23 AM by SYSTEM
Analysis Method : C:\USERS\PUBLIC\DOCUMENTS\CHEMSTATION\1\METHODS\Purity_195-315.M
Last changed    : 2/6/2023 2:02:18 PM by SYSTEM
Method Info     : OPERATOR: Organic QC lab
                  General gradient method starting @100% water for 1 min @0.3 ml/min, the 100%
                  Acetonitrile in 13 min, 100% Acetonitrile until T=16 min. Column Zorbax Eclipse
                  plus C-18, 2.1mmx50mm, 1.8 µm particle size. Agilent 1290 Infinity II LC/MS
                  system, Agilent 6125 quadrupole MS detector.
=====

```

Additional Info : Peak(s) manually integrated

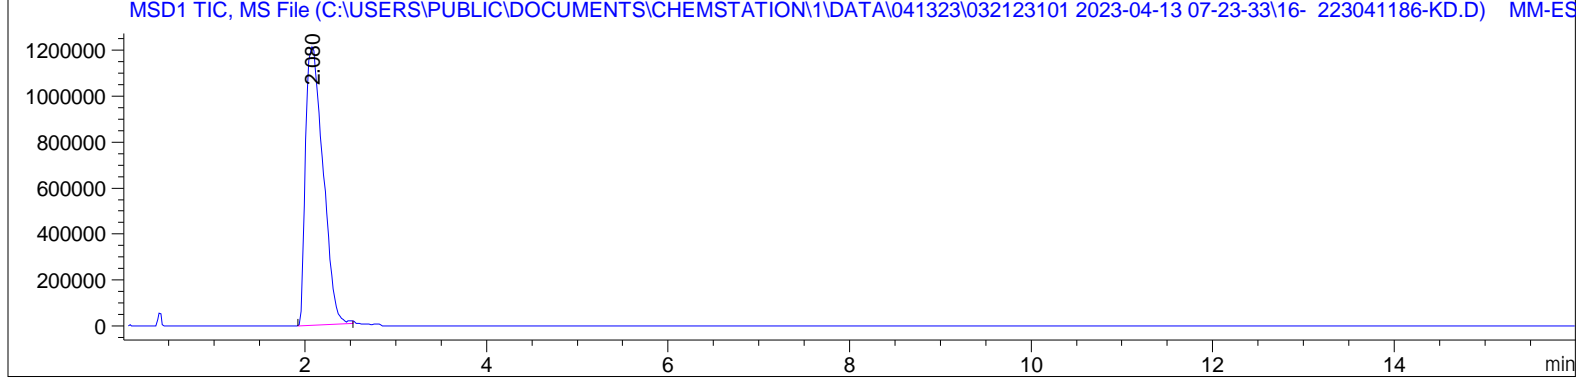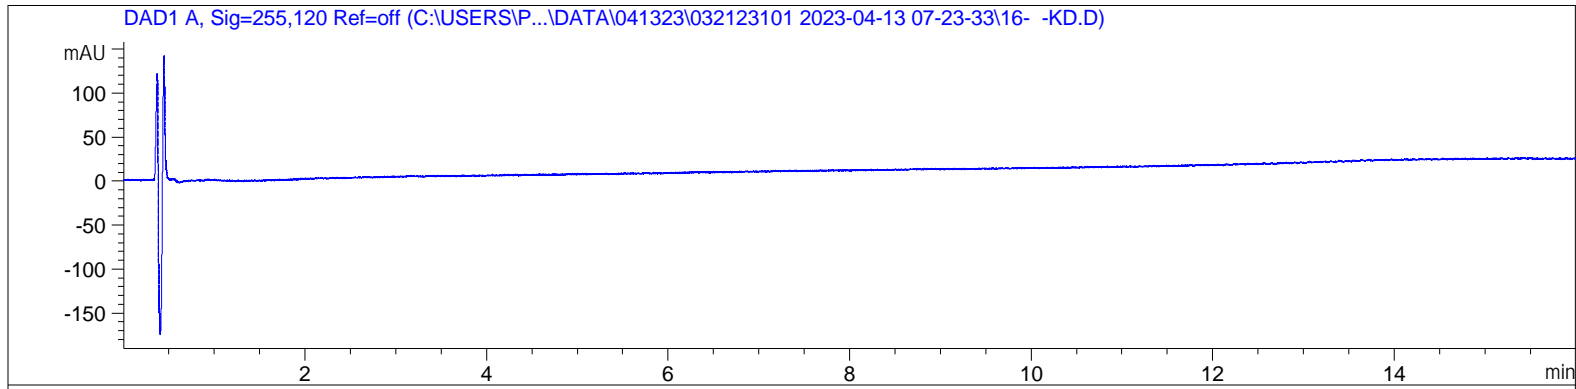

```

=====
                          Area Percent Report
=====

```

```

Sorted By      :      Signal
Multiplier     :      1.0000
Dilution      :      1.0000
Use Multiplier & Dilution Factor with ISTDs

```

Signal 1: DAD1 A, Sig=255,120 Ref=off

Signal 2: MSD1 TIC, MS File

Peak #	RetTime [min]	Type	Width [min]	Area	Height	Area %
1	2.080	BB	0.2057	1.63367e7	1.21177e6	100.0000

Totals : 1.63367e7 1.21177e6

=====
*** End of Report ***