File :Q:\GCMS-07 Minimal\DATA\05062002\44- .D
Operator : Organic QC department
Acquired : 07 May 20 07:01 am using AcqMethod KERLA-2Split-2uL.M
Instrument : 5977B MSD
Sample Name: PFRS-008S
Misc Info : Isodecyl diphenyl phosphate in Toluene
Vial Number: 137

AccuStandard®
Leader in Analytical Reference Standards
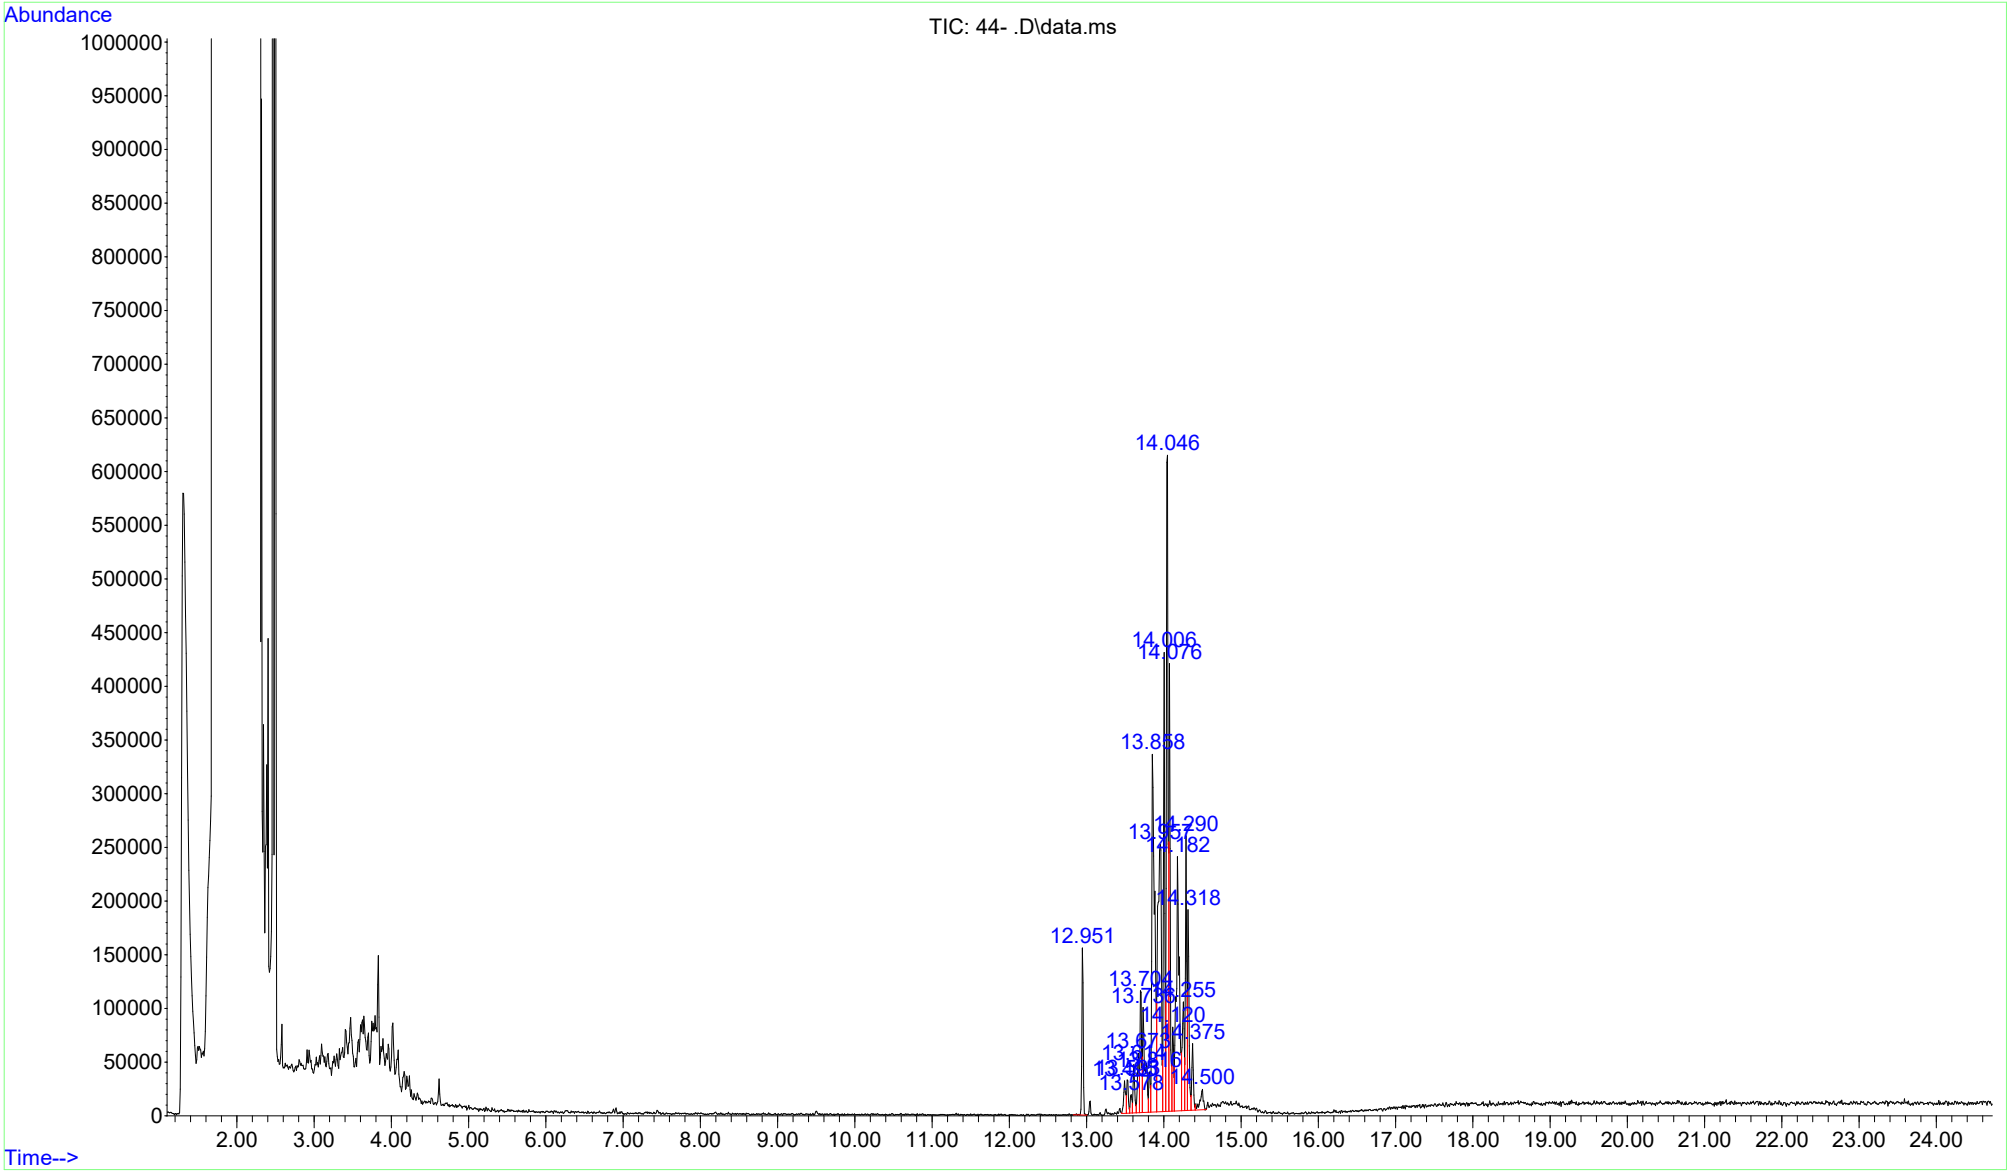
Column: DB-5MS, 30m, 0.25 ID, 0.25 um
Oven Program: 80c, 17c/min to 340c, 8min
GC Parameters: Cons. Split, 12psi constant flow
Split 2:1, 2uL inj.; GC/MS; INJ 270c