


File : L:\QC Data\GCMS-06 Minimal\DATA\052423\08 -SAK.D
Operator : Organic QC Lab
Acquired : 24 May 2023 11:45 using AcqMethod CHICK_2019_VOC-SV_S100.M
Instrument : GCMS 6
Sample Name: SDF-2X-100ML
Misc Info :
Vial Number: 116



Column: DB-5MS UI, 30m x 0.25mm ID x 0.25µm
Oven Program: 35°C, 17°C/min to 340°C (hold 8min)
GC Parameters: Pulsed split 40psi 0.5min, 10psi constant flow
Split 20:1, 1µl inj.; GC/MS; Injector temp 270°C

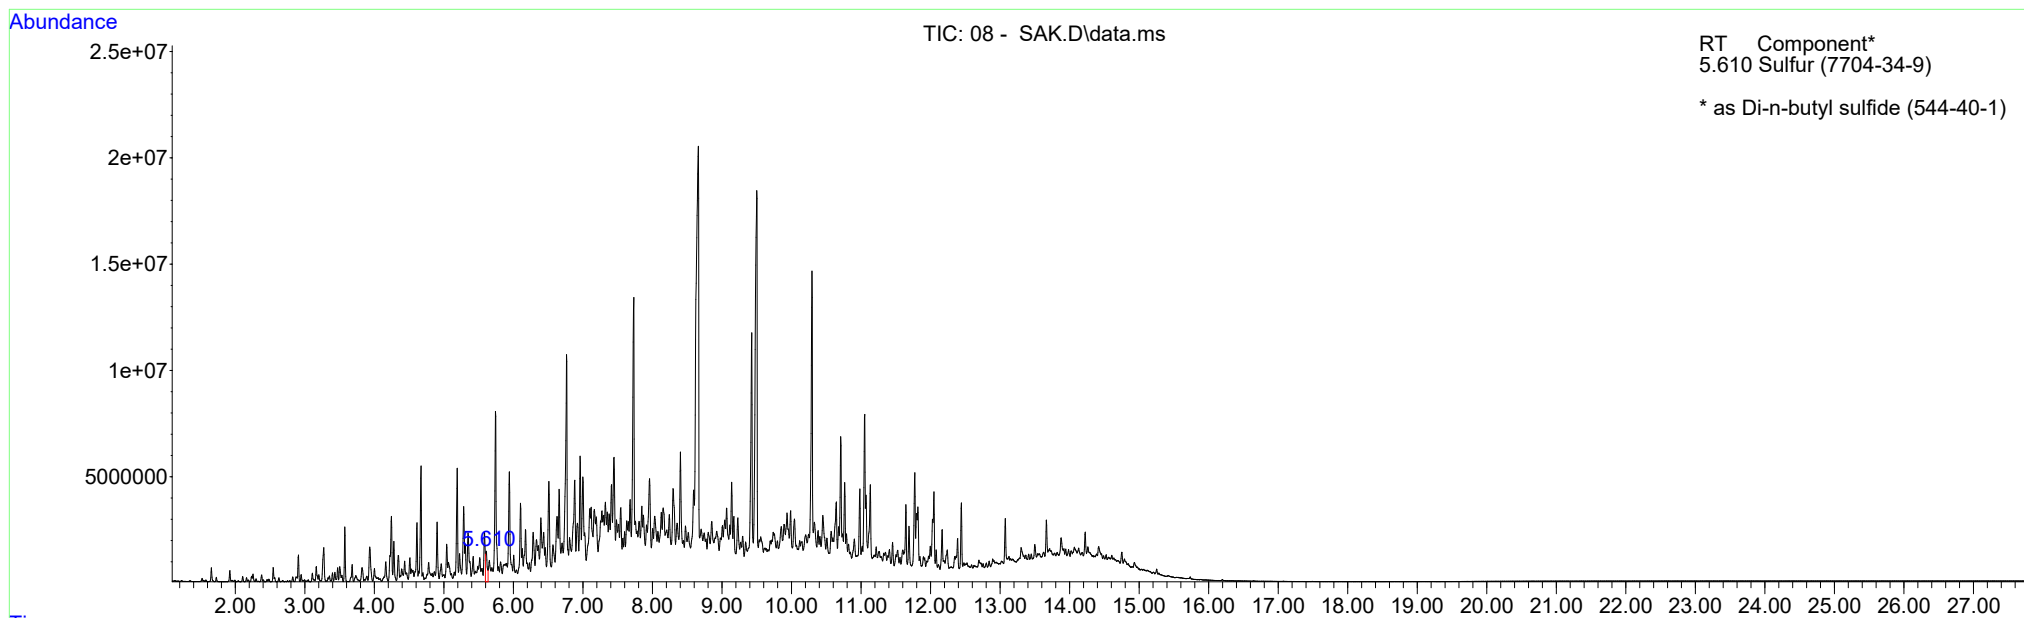

RT Component*
5.610 Sulfur (7704-34-9)
* as Di-n-butyl sulfide (544-40-1)

