


File :Q:\GCMS-08 Minimal\DATA\20230410\30- (JP).D
Operator : Organic QC Lab
Acquired : 10 Apr 23 09:17 pm using AcqMethod Hy_Pest_15cm_S2_3ulinj.M
Instrument : GCMS 8
Sample Name: C-CSA-05
Misc Info : PCB's in iso
Vial Number: 4



Column: DB-5MS UI, 30m x 0.25mm ID x 0.25µm
Oven Program: 80°C, 17°C/min to 340°C (hold 8min)
GC Parameters: Pulsed split 40psi 0.5min, 10psi constant flow
Split 2:1, 2µl inj.; GC/MS; Injector 270°C

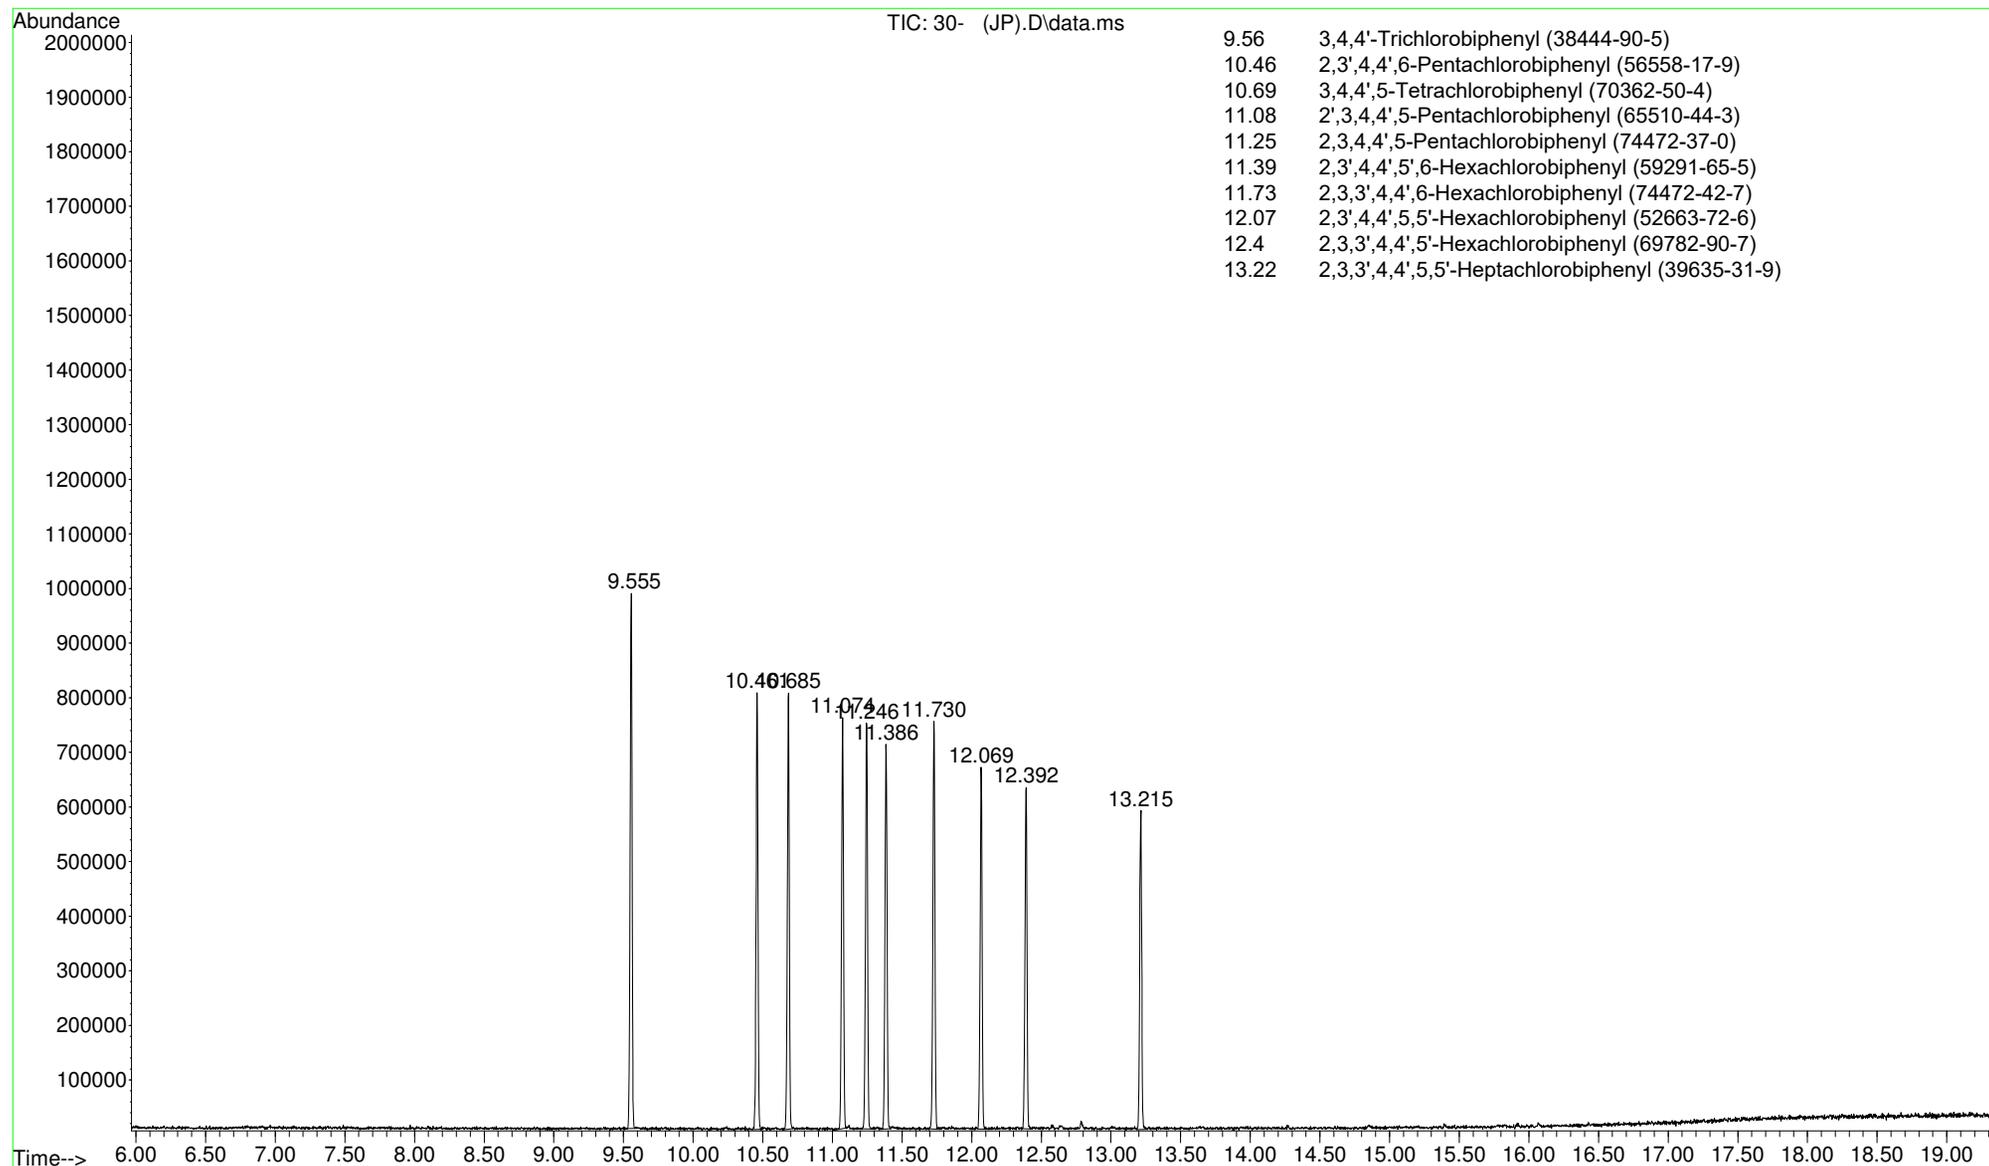

9.56	3,4,4'-Trichlorobiphenyl (38444-90-5)
10.46	2,3',4,4',6-Pentachlorobiphenyl (56558-17-9)
10.69	3,4,4',5-Tetrachlorobiphenyl (70362-50-4)
11.08	2',3,4,4',5-Pentachlorobiphenyl (65510-44-3)
11.25	2,3,4,4',5-Pentachlorobiphenyl (74472-37-0)
11.39	2,3',4,4',5',6-Hexachlorobiphenyl (59291-65-5)
11.73	2,3,3',4,4',6-Hexachlorobiphenyl (74472-42-7)
12.07	2,3',4,4',5,5'-Hexachlorobiphenyl (52663-72-6)
12.4	2,3,3',4,4',5'-Hexachlorobiphenyl (69782-90-7)
13.22	2,3,3',4,4',5,5'-Heptachlorobiphenyl (39635-31-9)