Print of window 38: Current Chromatogram(s)
Data File : D:\DATA\09132023\16-KD.D
Sample Name : CP-FL-01

==========

Acq. Operator : SYSTEM Seq. Line : 6
Acq. Instrument : LCMS-1 Location : P1-F6
Injection Date : 9/13/2023 11:05:20 AM Inj : 1
Inj Volume : 1.000 µl

Acq. Method : C:\CHEM32\1\METHODS\Purity195_315.M
Last changed : 1/5/2023 12:01:53 PM by SYSTEM
Analysis Method : C:\CHEM32\1\METHODS\Purity195_315.M
Last changed : 9/15/2023 8:27:06 AM by SYSTEM
(modified after loading)
Method Info : Operator: Organic QC lab
Gradient Method Starting @ 100 % Water/0 % Acetonitrile to 0 % Water/100 % Acetonitrile in 13 min, then 3 min at 100/0, post-run time 2 min. Flow rate :0.3 ml/min, column Zorbax Eclipse Plus C-18, 2.1x50 mm, 1.8 micron particle size. Agilent 1290 Infinity II LC system, Agilent 6120 Quadrople MS Detector. No UV Reference.

Current Chromatogram(s)

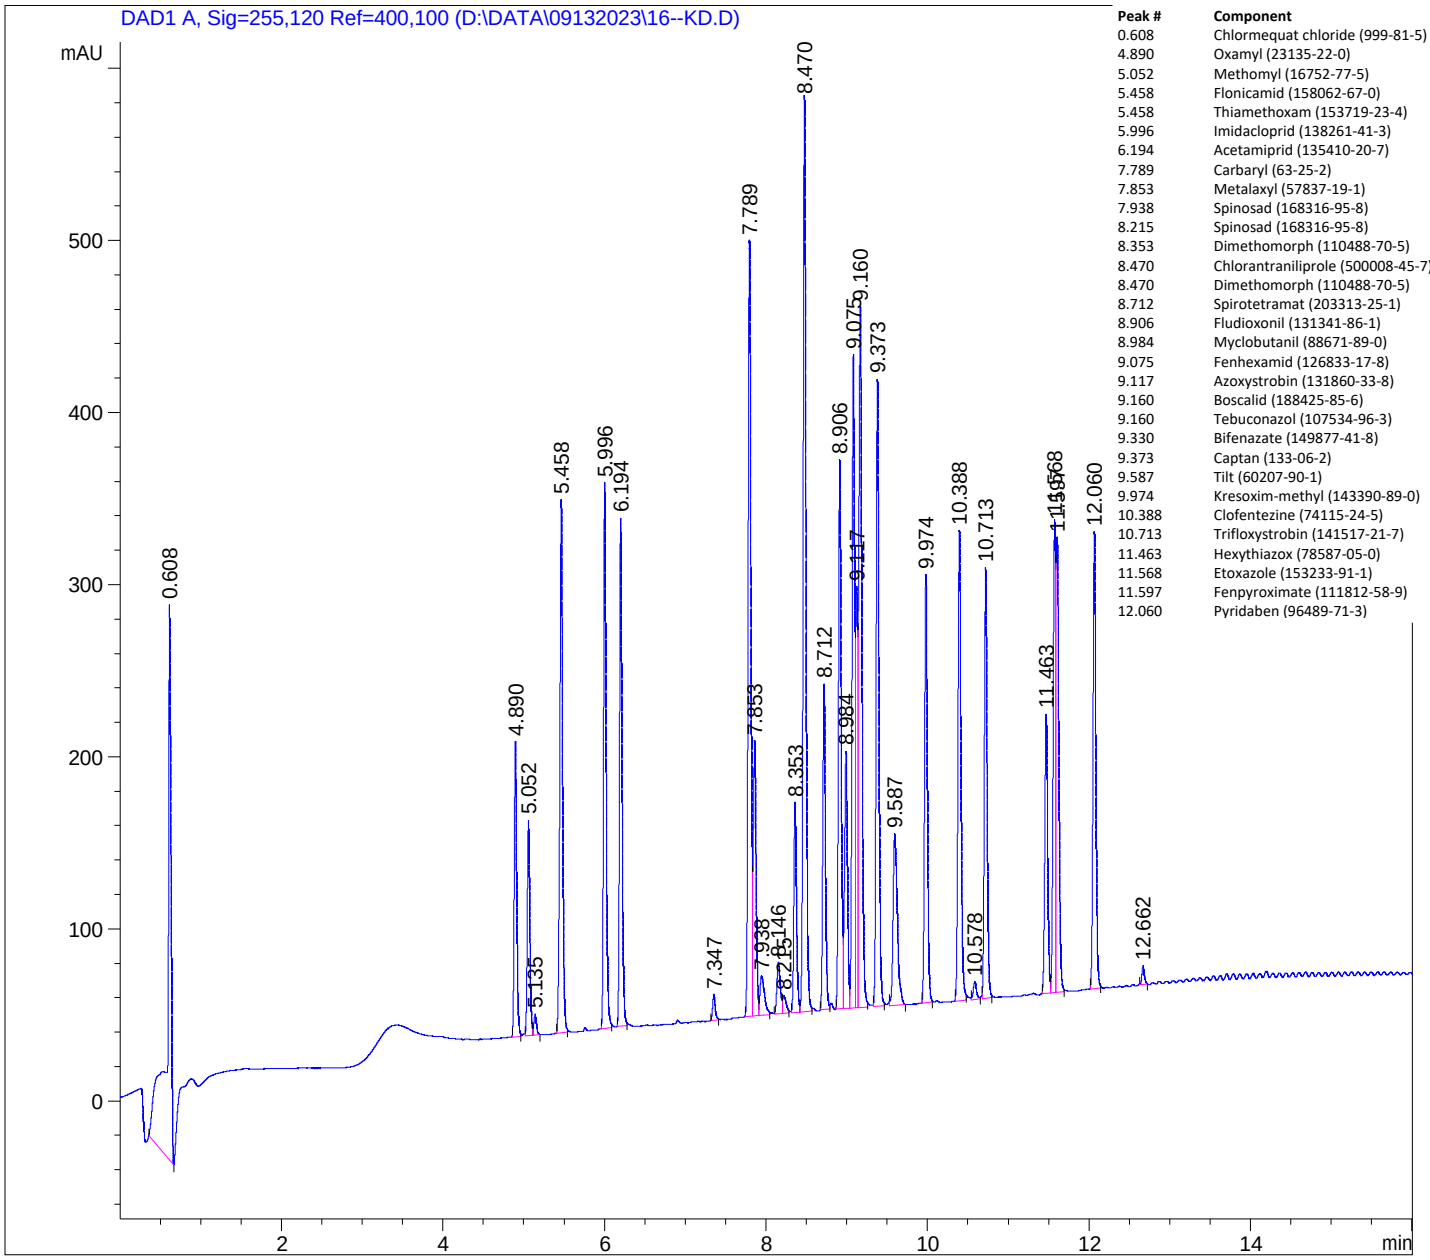

Peak #	Component
0.608	Chlormequat chloride (999-81-5)
4.890	Oxamyl (23135-22-0)
5.052	Methomyl (16752-77-5)
5.458	Flonicamid (158062-67-0)
5.458	Thiamethoxam (153719-23-4)
5.996	Imidacloprid (138261-41-3)
6.194	Acetamiprid (135410-20-7)
7.789	Carbaryl (63-25-2)
7.853	Metalaxyl (57837-19-1)
7.938	Spinosad (168316-95-8)
8.215	Spinosad (168316-95-8)
8.353	Dimethomorph (110488-70-5)
8.470	Chlorantraniliprole (500008-45-7)
8.470	Dimethomorph (110488-70-5)
8.712	Spirotetramat (203313-25-1)
8.906	Fludioxonil (131341-86-1)
8.984	Myclobutanil (88671-89-0)
9.075	Fenhexamid (126833-17-8)
9.117	Azoxystrobin (131860-33-8)
9.160	Boscalid (188425-85-6)
9.160	Tebuconazol (107534-96-3)
9.330	Bifenazate (149877-41-8)
9.373	Captan (133-06-2)
9.587	Tilt (60207-90-1)
9.974	Kresoxim-methyl (143390-89-0)
10.388	Clofentezine (74115-24-5)
10.713	Trifloxystrobin (141517-21-7)
11.463	Hexythiazox (78587-05-0)
11.568	Etoxazole (153233-91-1)
11.597	Fenpyroximate (111812-58-9)
12.060	Pyridaben (96489-71-3)