Print of window 38: Current Chromatogram(s)
Data File : C:\USERS\P...ION\1\DATA\101023\101023101 2023-10-10 16-37-32\36- ALR.D
Sample Name : DYE-023S-R1

==========

Acq. Operator : SYSTEM Seq. Line :
Sample Operator : SYSTEM
Acq. Instrument : LCMS-2 Location : P2-D-02
Injection Date : 10/11/2023 3:38:16 AM Inj : 1
Inj Volume : 1.000 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 2.000 µl
Acq. Method : C:\Users\Public\Documents\ChemStation\1\Data\101023\101023101 2023-10-10 16-37-32 \Purity_195-315.M
Last changed : 2/6/2023 2:02:18 PM by SYSTEM
Analysis Method : C:\Users\Public\Documents\ChemStation\1\Methods\Purity_195-315.M
Last changed : 2/6/2023 2:02:18 PM by SYSTEM
Method Info : OPERATOR: Organic QC lab
General gradient method starting @100% water for 1 min @0.3 ml/min,the 100% Acetonitile in 13 min, 100% Acetonitrile until T=16 min. Column Zorbax Eclipse plus C-18, 2.1mmx50mm, 1.8 u particlue size. Agilent 1290 Infinity II LC/MS system , Agilent 6125 quadrupole MS detector.

Sample Info : Solvent Red 24 in MeOH/DCM 95/5

Additional Info : Peak(s) manually integrated
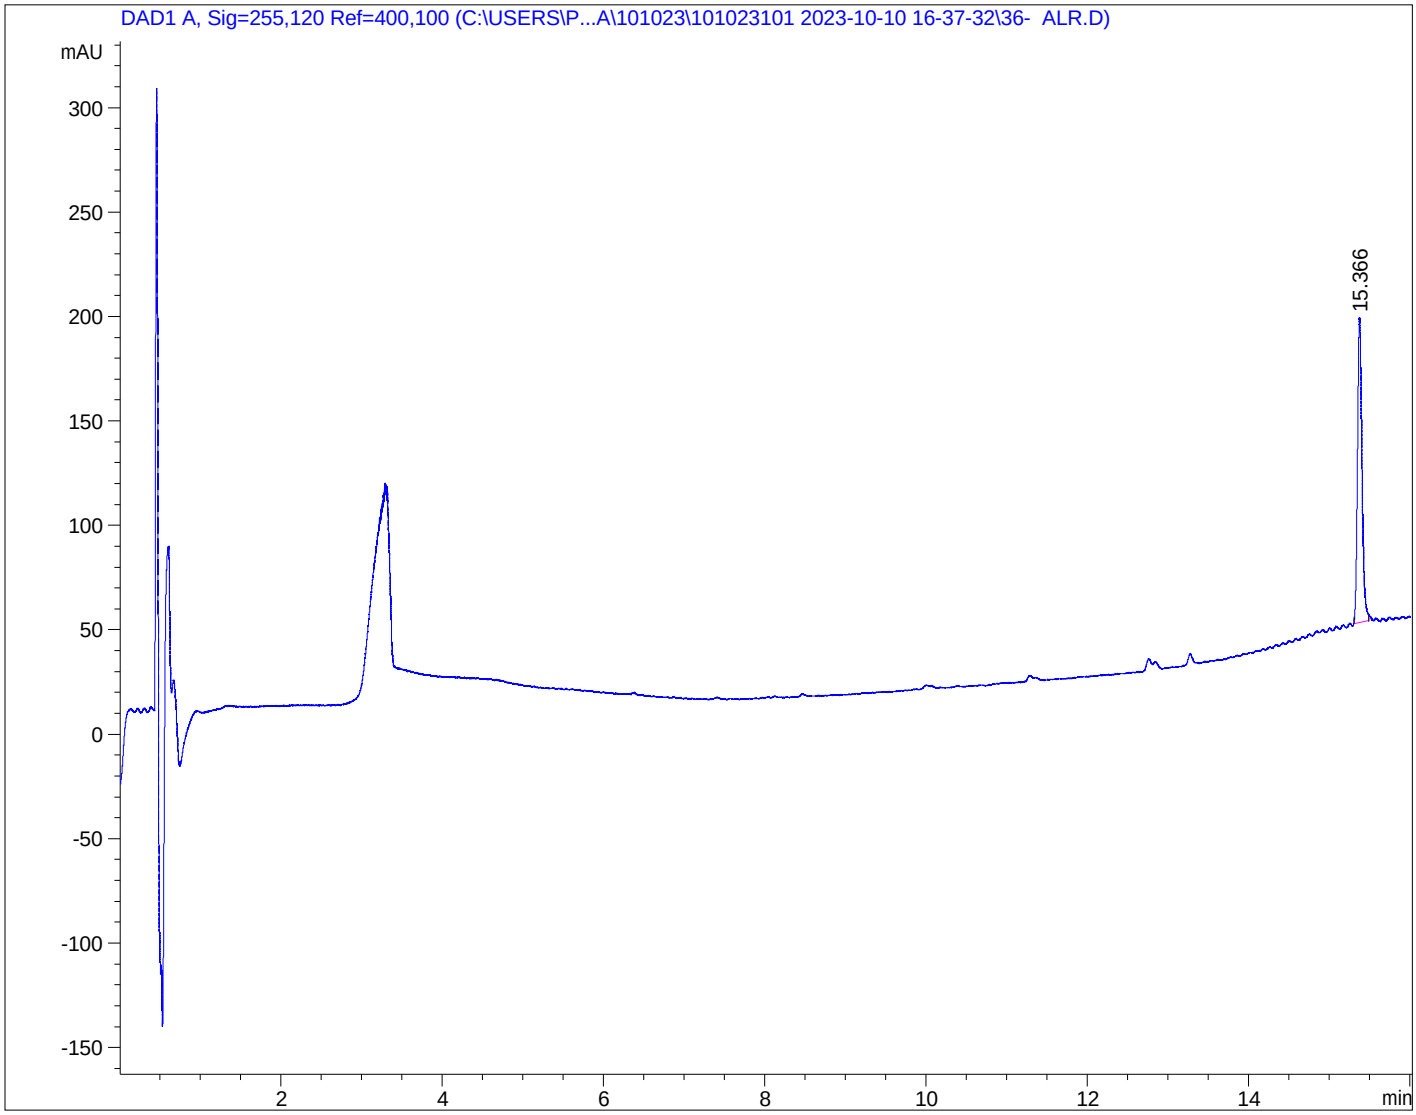
Current Chromatogram(s)