File :Q:\GCMS-08 Minimal\DATA\20191212\11a- .D
Operator :
Acquired : 12 Dec 2019 14:54 using AcqMethod Pest_15cm_S1.M
Instrument : GCMS 8
Sample Name: M-1618-4
Misc Info : in isooctane
Vial Number: 53

AccuStandard®
Leader in Analytical Reference Standards
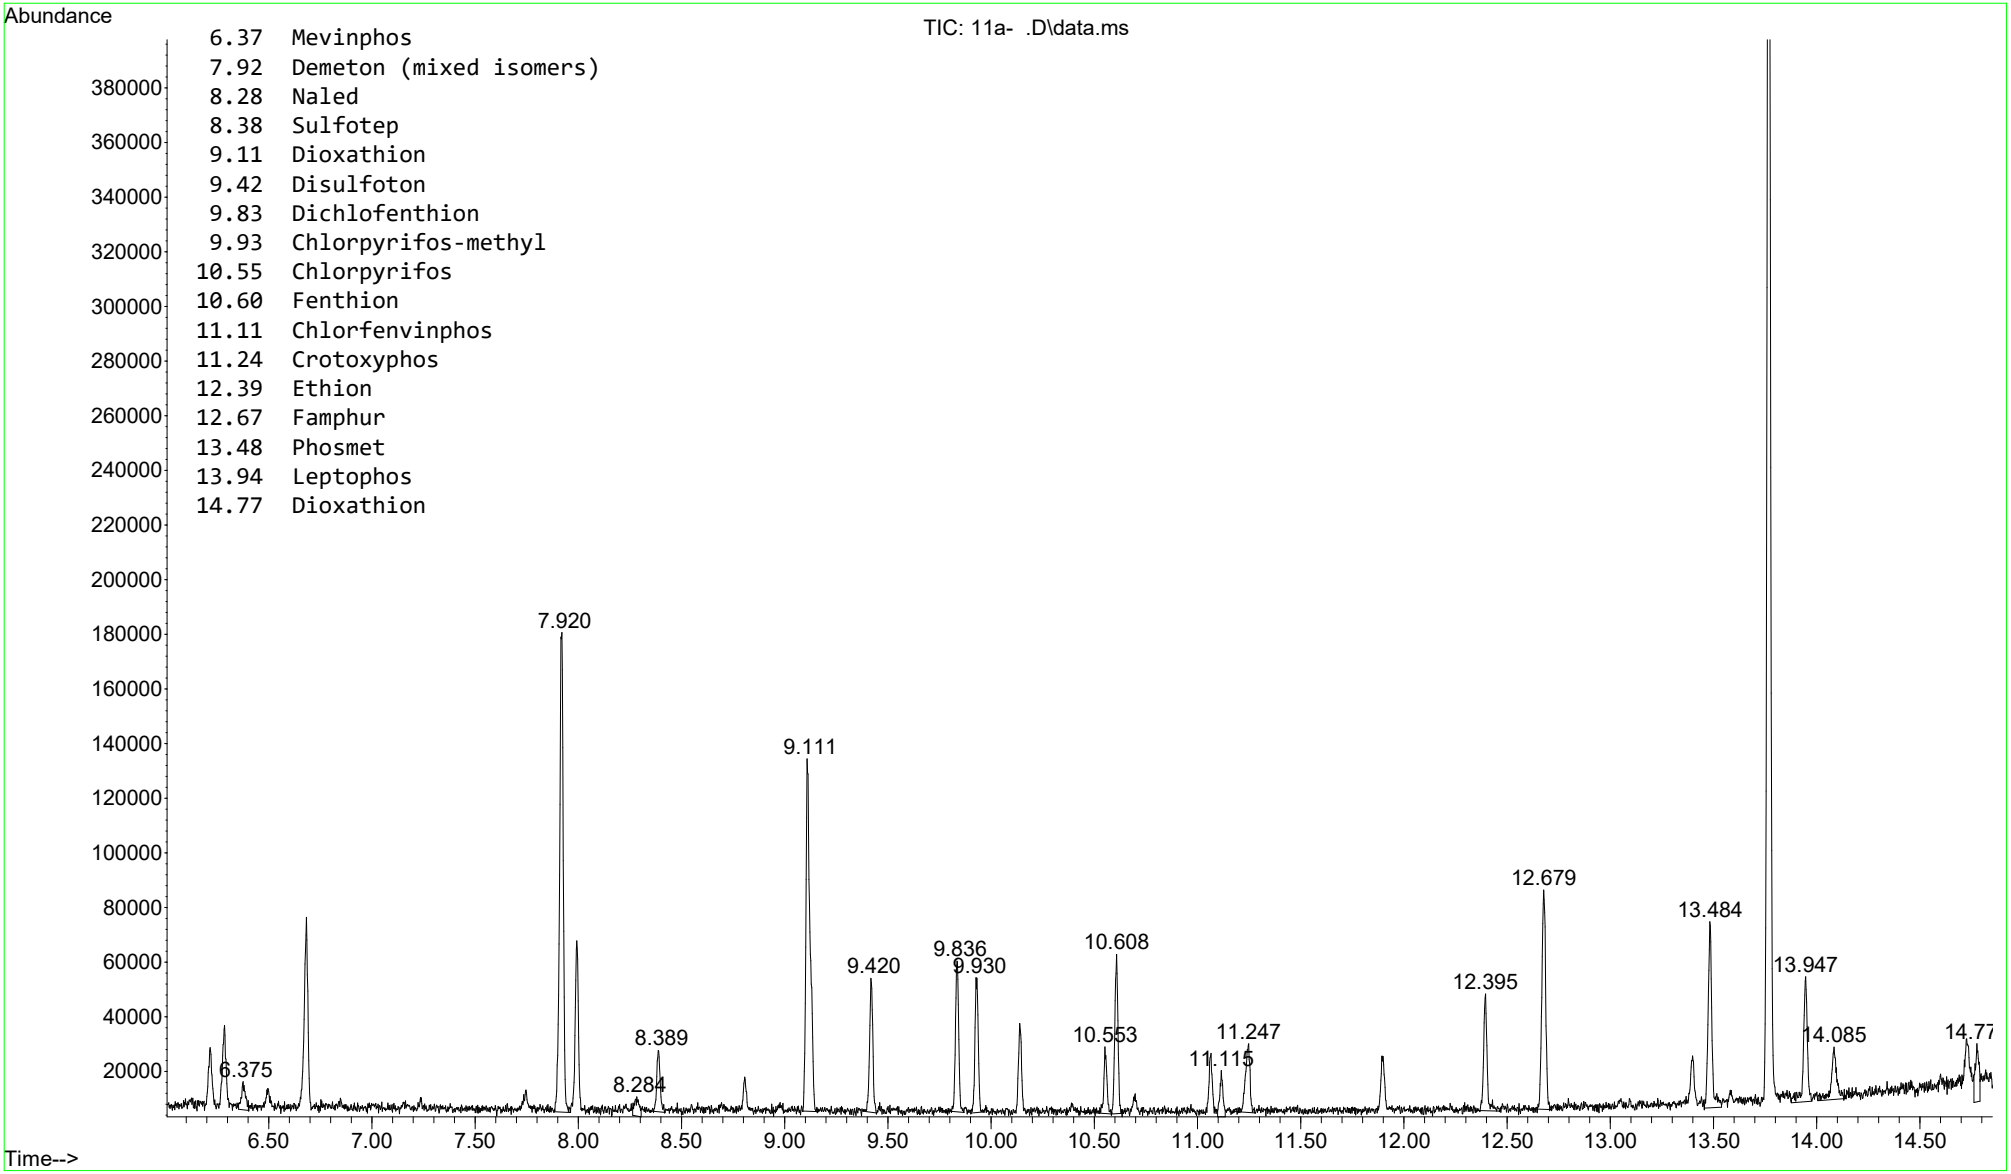
Column: DB-5, 30m, 0.25 ID, 0.25um
Oven Program: 80c, 1m, 15c/min to 340c, final 2min.
GC Parameters: Split 1:1, 3ul inj.; GC/MS; INJ 270c.