


File :Q:\GCMS-06 Minimal\DATA\011421\BSB\15- KM.D
Operator : Organic QC Lab
Acquired : 14 Jan 2021 14:56 using AcqMethod CHICK_2019_2S_2uL.M
Instrument : GCMS 6
Sample Name: M-515-QC-R
Misc Info : Calibration Solution in MtBE
Vial Number: 38



Column: DB-5MS UI, 30m x 0.25mm ID x 0.25µm
Oven Program: 80°C, 17°C/min to 340°C (hold 8min)
GC Parameters: Pulsed split 40psi 0.5min, 10psi constant flow
Split 20:1, 1µl inj.; GC/MS; Injector 270°C

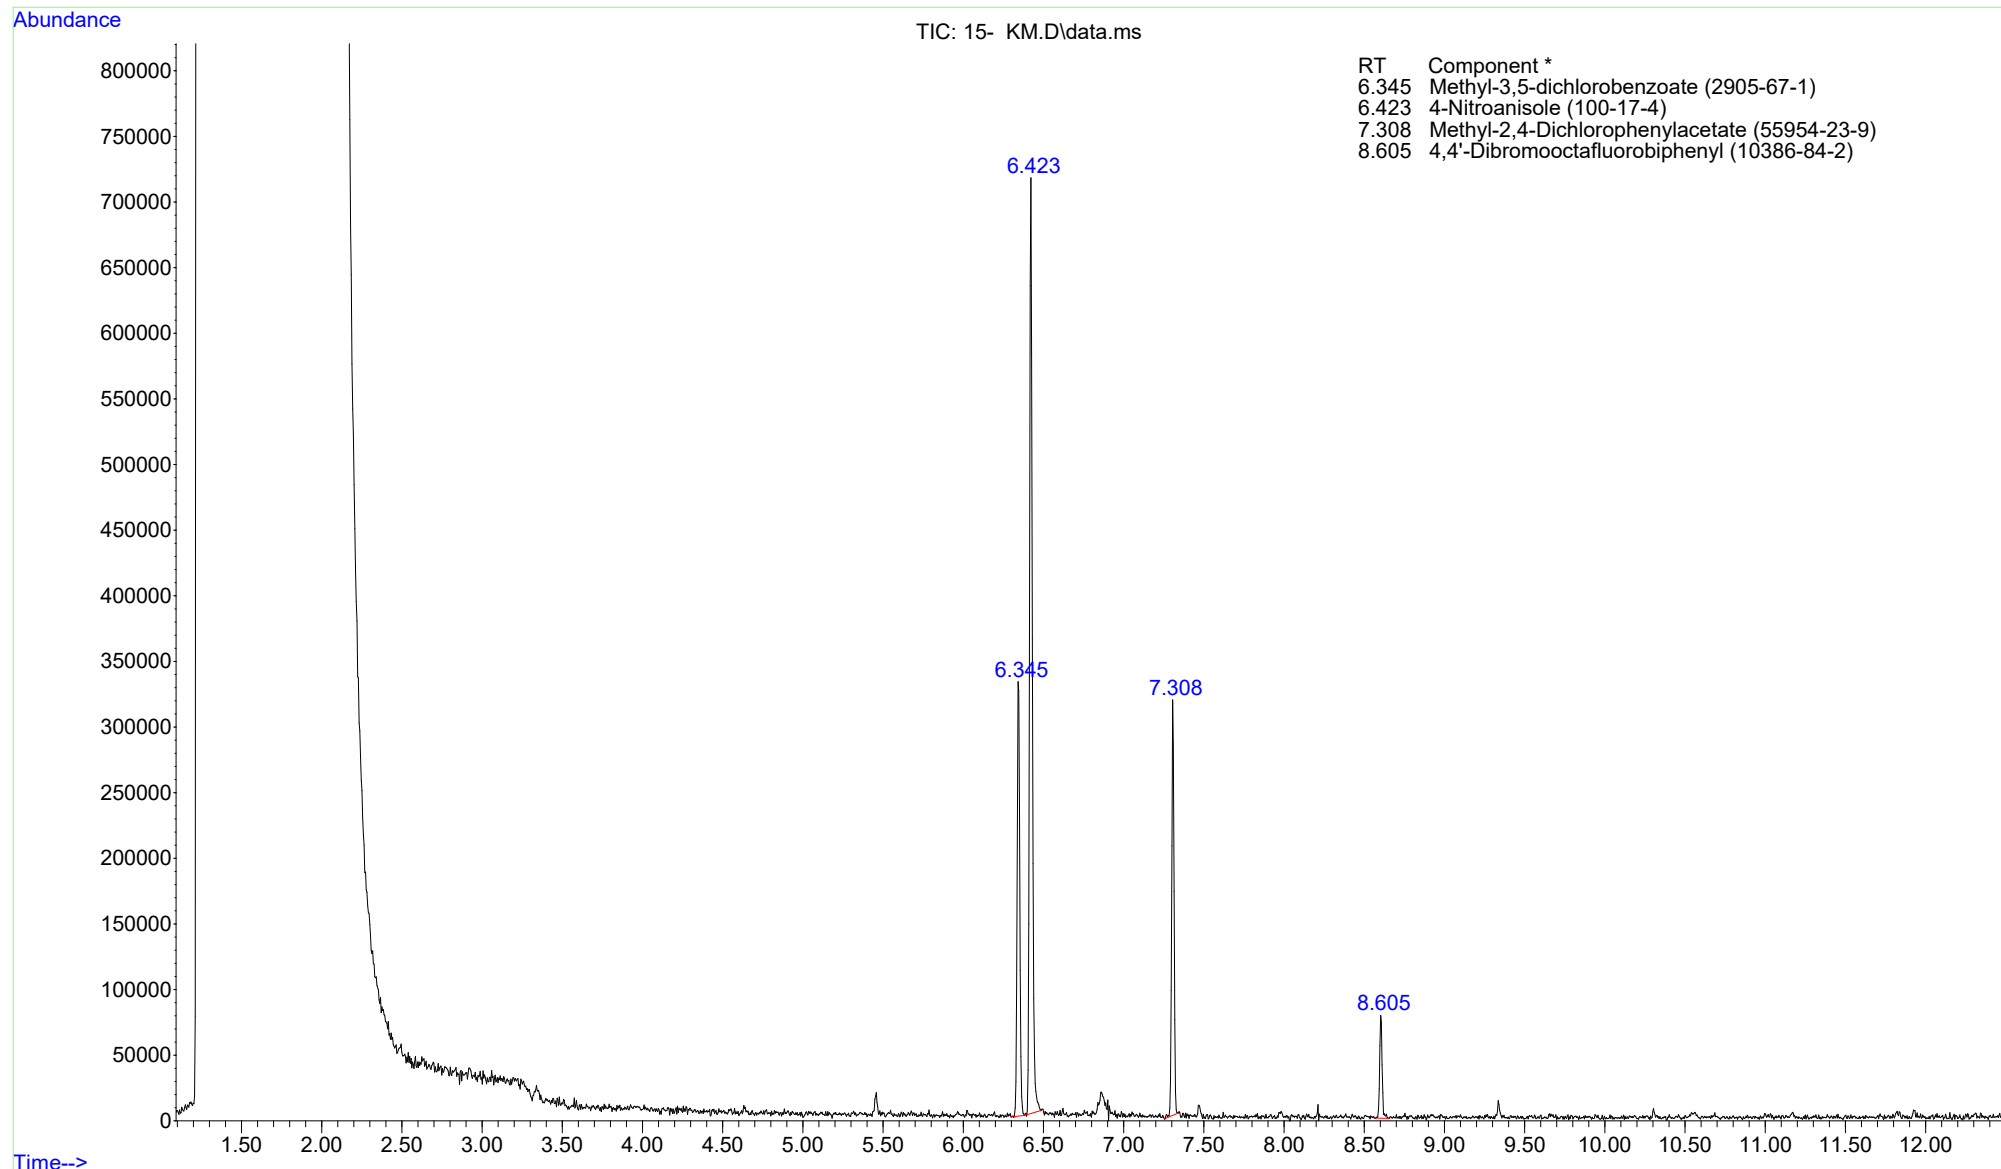

* Dinoseb methyl ether (6099-79-2) not seen at this concentration