


File :Q:\GCMS-08 Minimal\DATA\20191107\21- .D
Operator : KM / JP / ZA
Acquired : 07 Nov 2019 20:05 using AcqMethod KERLA-VOC-SV.M
Instrument : GCMS 8
Sample Name: M-552A-R-03
Misc Info : Chloroacetic acid in MtBE Derivatized
Vial Number: 19



AccuStandard®

Column: DB-5MS UI, 30m x 0.25mm ID x 0.25µm
Oven Program: 80°C, 17°C/min to 340°C (hold 8min)
GC Parameters: Pulsed split 40psi 0.5min, 10psi constant flow
Split 20:1, 1µl inj.; GC/MS; Injector 270°C

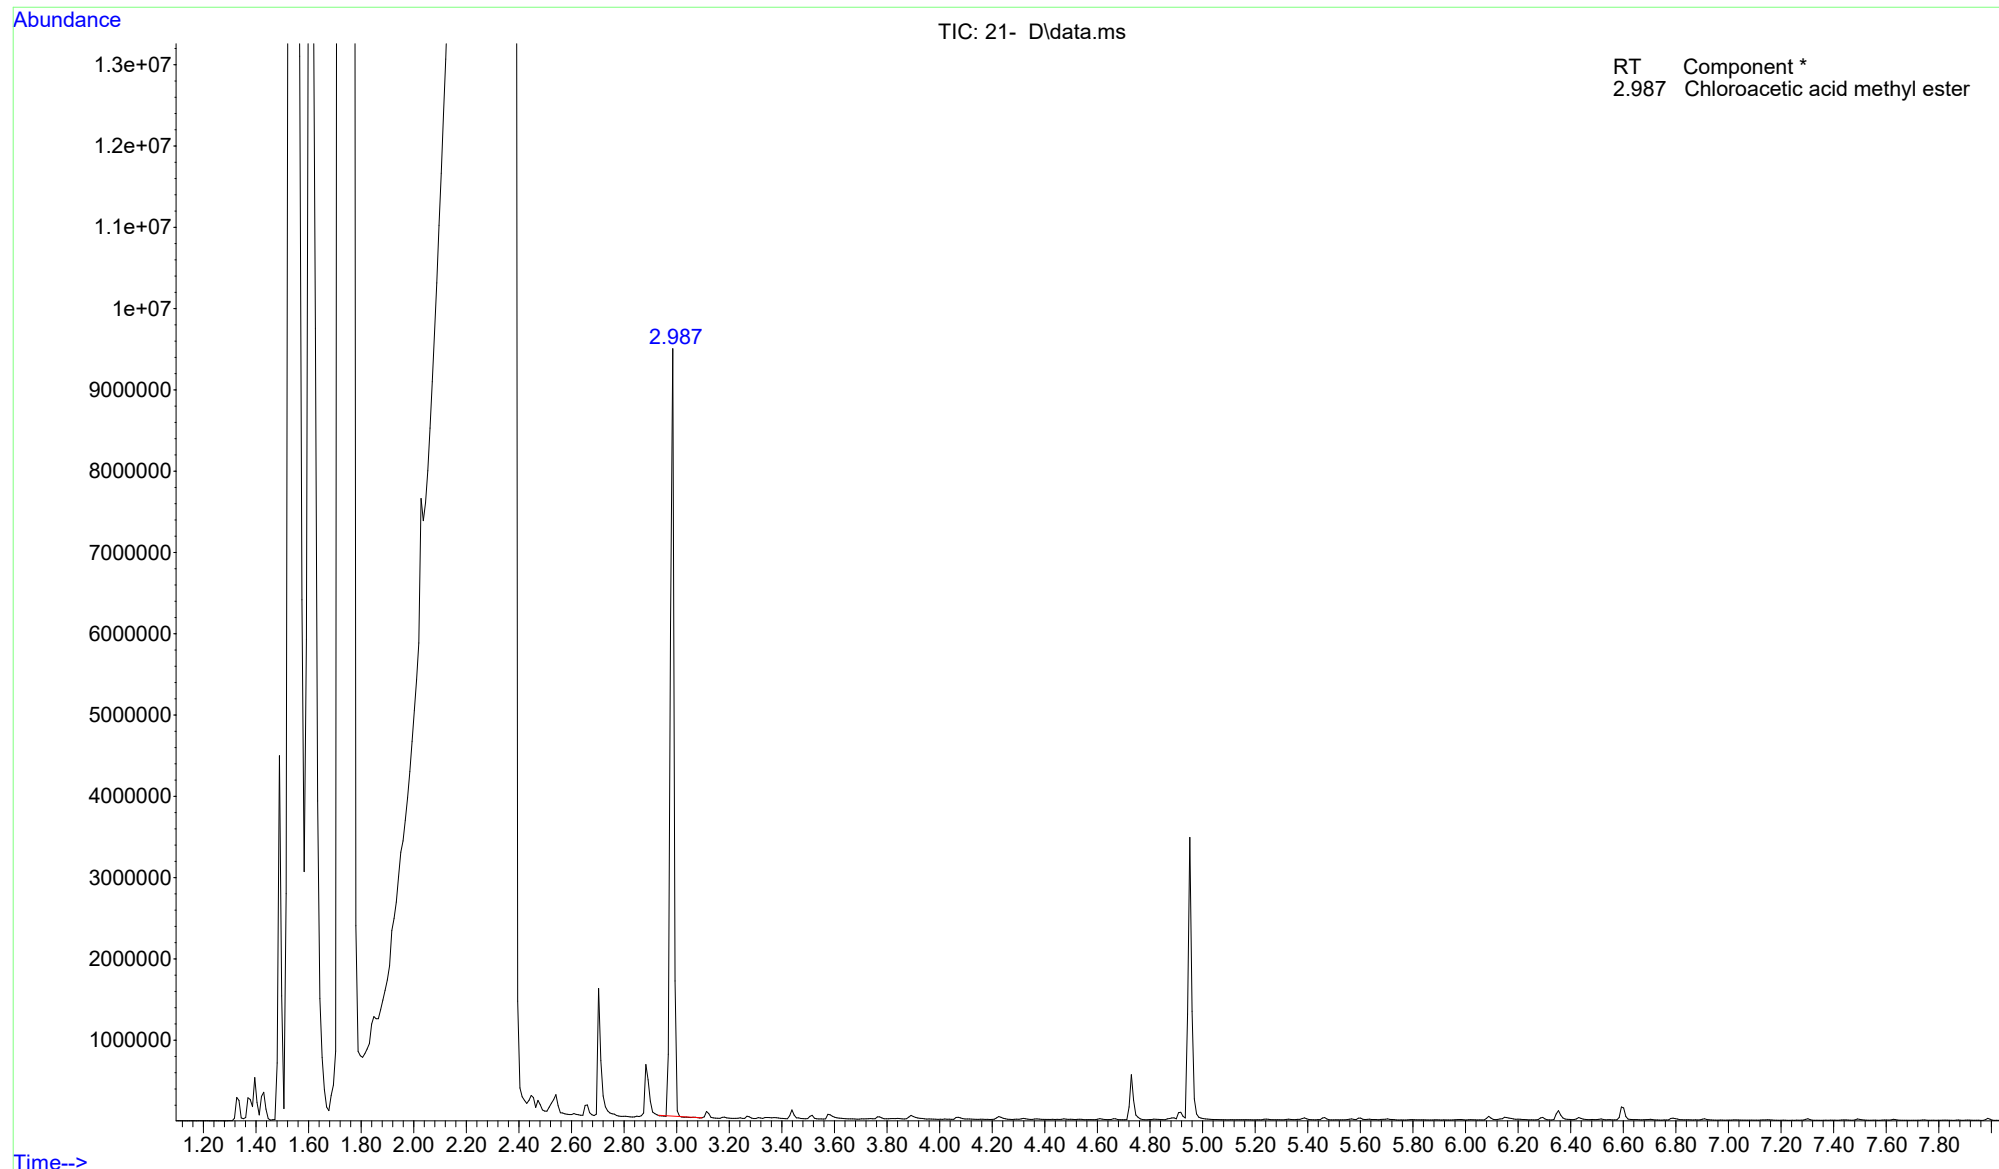

* Derivatized in diazomethane to form methyl ester