Print of window 38: Current Chromatogram(s)
Data File : C:\USERS\P...N\1\DATA\02132301\021323101 2023-02-13 06-54-18\03-KD.D
Sample Name : M-554-DNPH-02

==========

Acq. Operator : SYSTEM Seq. Line : 3
Sample Operator : SYSTEM
Acq. Instrument : LCMS-2 Location : P1-C-08
Injection Date : 2/13/2023 7:29:03 AM Inj : 1
Inj Volume : 1.000 µl
Acq. Method : C:\Users\Public\Documents\ChemStation\1\Data\02132301\021323101 2023-02-13 06-54-18\DNPH.M
Last changed : 12/4/2019 12:27:07 PM by SYSTEM
Analysis Method : C:\Users\Public\Documents\ChemStation\1\Data\01302301\013023101 2023-01-30 06-52-36\Purity_195-315.M (Sequence Method)
Last changed : 3/23/2022 11:04:54 AM by SYSTEM
Method Info : OPERATOR: Organic QC lab
General gradient method starting @100% water for 1 min @0.3 ml/min,the 100% Acetonitile in 13 min, 100% Acetonitrile until T=16 min. Column Zorbax Eclipse plus C-18, 2.1mmx50mm, 1.8 u particlue size. Agilent 1290 Infinity II LC/MS system, Agilent 6125 quadrupole MS detector.

Sample Info : diluted in ACCN

Additional Info : Peak(s) manually integrated
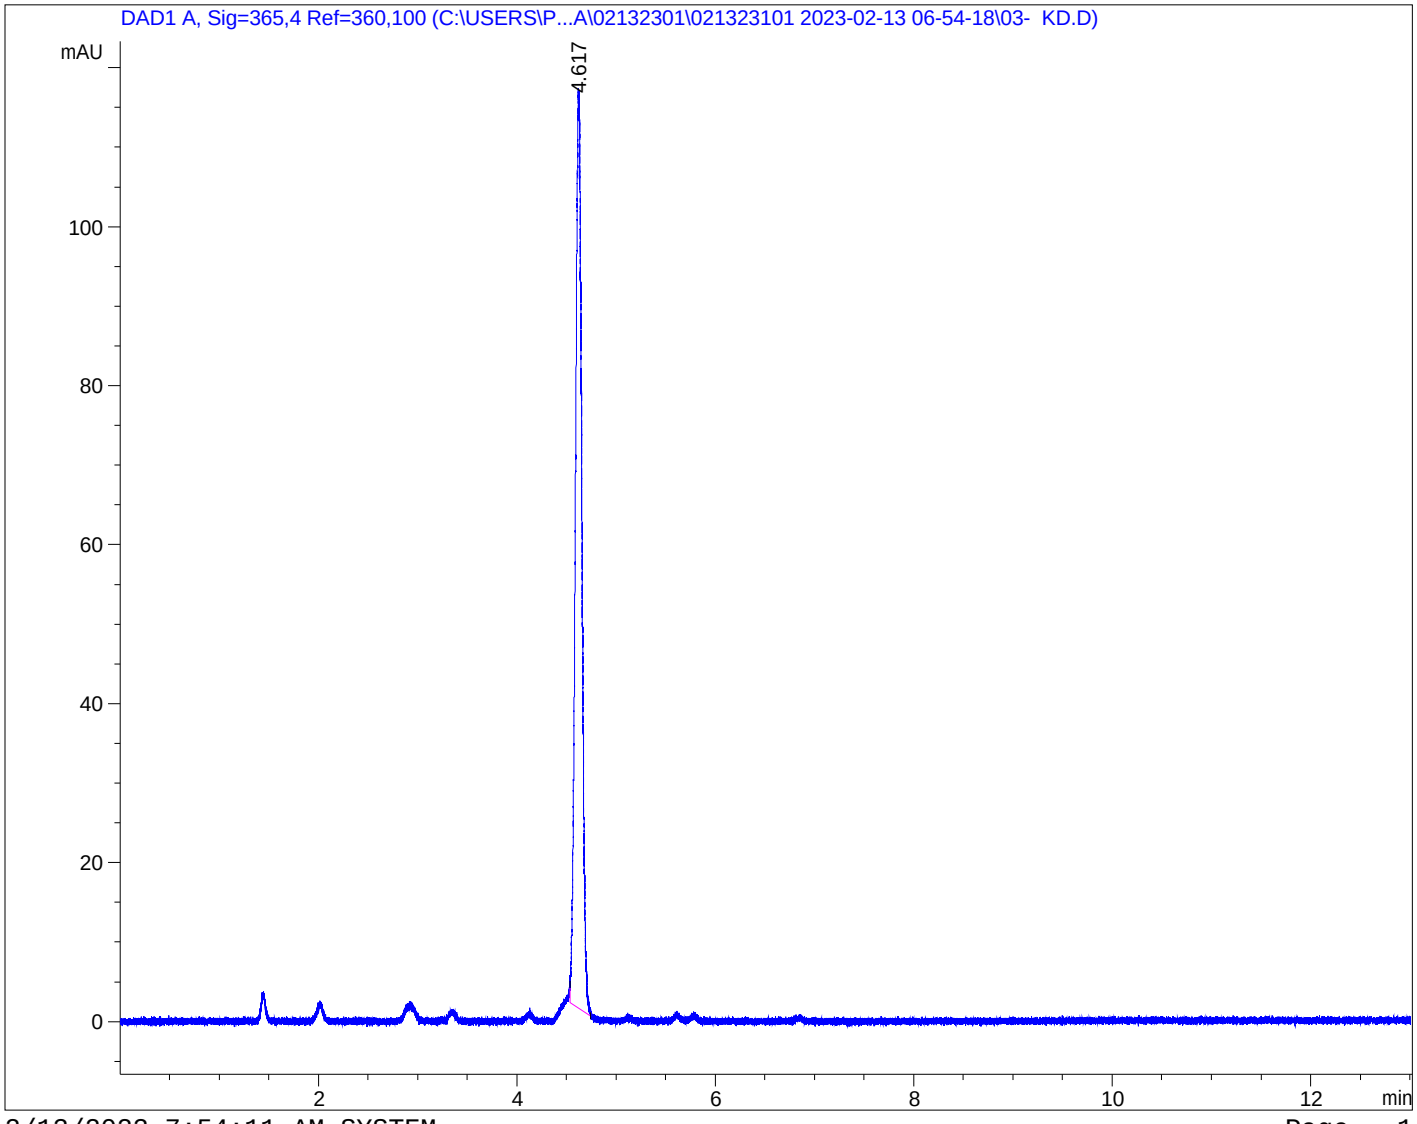
Current Chromatogram(s)