Print of window 38: Current Chromatogram(s)
Data File : C:\USERS\P...ON\1\DATA\07262101\07232101 2021-07-26 06-51-58\04- -KD.D
Sample Name : M-8315-R-DNPH-01-0.1X

==========

Acq. Operator : SYSTEM Seq. Line : 4
Sample Operator : SYSTEM
Acq. Instrument : LCMS-2 Location : P1-A-03
Injection Date : 7/26/2021 7:49:53 AM Inj : 1
Inj Volume : 1.000 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 2.000 µl
Acq. Method : C:\Users\Public\Documents\ChemStation\1\Data\07262101\07232101 2021-07-26 06-51-58 \Purity_195-315.M
Last changed : 4/29/2021 10:41:07 AM by SYSTEM
Analysis Method : C:\Users\Public\Documents\ChemStation\1\Methods\Purity_195-315.M
Last changed : 4/29/2021 10:41:07 AM by SYSTEM
Method Info : OPERATOR: Organic QC lab
General gradient method starting @100% water for 1 min @0.3 ml/min,the 100% Acetonitile in 13 min, 100% Acetonitrile until T=16 min. Column Zorbax Eclipse plus C-18, 2.1mmx50mm, 1.8 u particlue size. Agilent 1290 Infinity II LC/MS system , Agilent 6125 quadrupole MS detector.

Additional Info : Peak(s) manually integrated
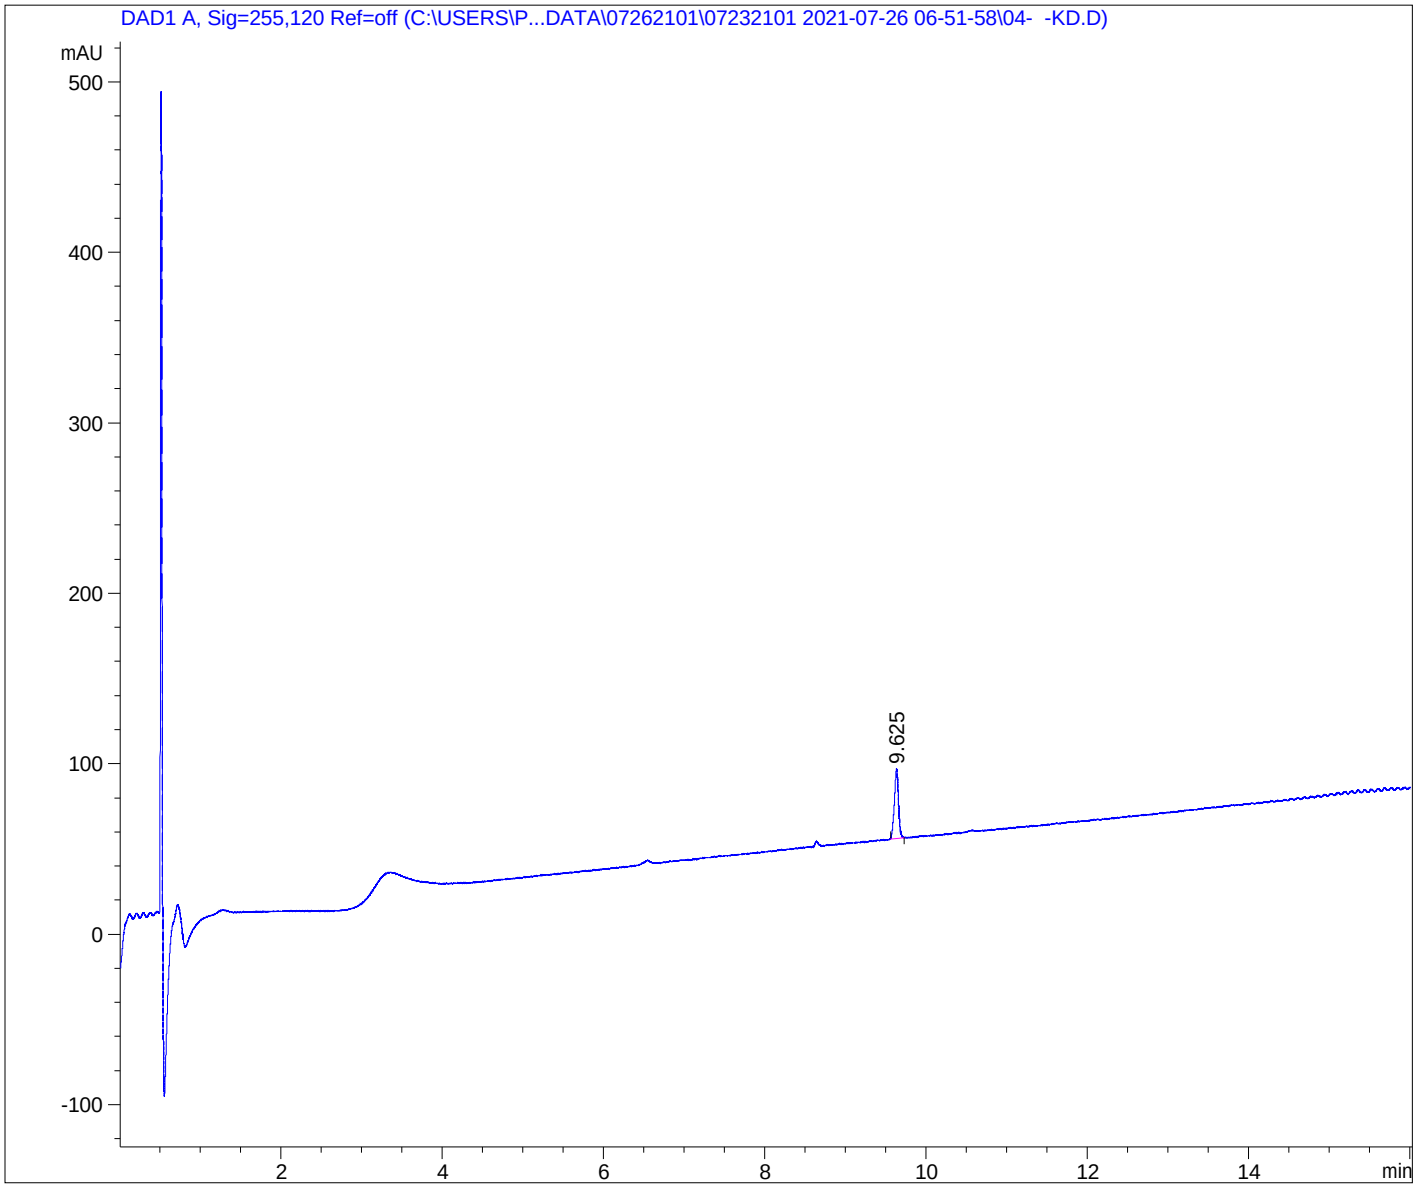
Current Chromatogram(s)