



Totals : 3.28593e6 5.38783e5

=====  
\*\*\* End of Report \*\*\*


Sample Name: M-8327-10X

```

=====
Acq. Operator   : SYSTEM                      Seq. Line :    4
Sample Operator : SYSTEM
Acq. Instrument : LCMS-2                      Location  : P2-A5
Injection Date  : 1/5/2024 8:23:54 AM        Inj       :    4
                                           Inj Volume: 2.000 µl

Acq. Method     : C:\Users\Public\Documents\ChemStation\1\Data\010524\010424 2024-01-05 07-
                26-34\PFAA.M
Last changed    : 1/26/2021 10:30:23 AM by SYSTEM
Analysis Method : C:\USERS\PUBLIC\DOCUMENTS\CHEMSTATION\1\METHODS\Purity_195-315.M
Last changed    : 2/6/2023 2:02:18 PM by SYSTEM
Method Info     : OPERATOR: Organic QC lab
                General gradient method starting @100% water for 1 min @0.3 ml/min, the 100
                % Acetonitrile in 13 min, 100% Acetonitrile until T=16 min. Column Zorbax
                Eclipse plus C-18, 2.1mmx50mm, 1.8 µm particle size. Agilent 1290 Infinity
                II LC/MS system, Agilent 6125 quadrupole MS detector.
=====

```

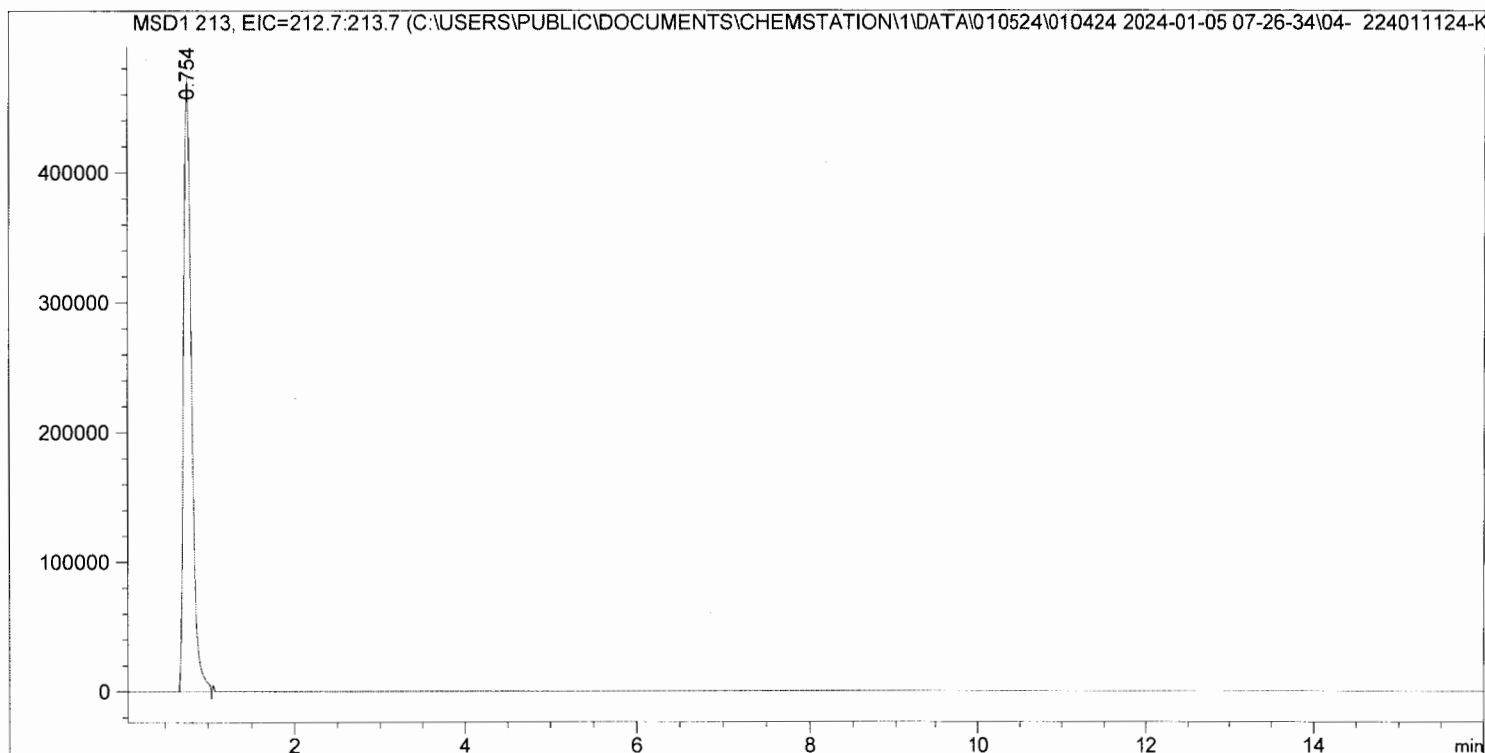

```

=====
                          Area Percent Report
=====

```

```

Sorted By           :      Signal
Multiplier          :      1.0000
Dilution            :      1.0000
Use Multiplier & Dilution Factor with ISTDs

```

Signal 1: MSD1 213, EIC=212.7:213.7

Peak #	RetTime [min]	Type	Width [min]	Area	Height	Area %
1	0.754	BV	0.1010	3.00751e6	4.73633e5	100.0000

Totals : 3.00751e6 4.73633e5

=====  
\*\*\* End of Report \*\*\*




Totals : 3.48308e6 5.83545e5

=====  
\*\*\* End of Report \*\*\*

```
=====
Acq. Operator   : SYSTEM                      Seq. Line :    6
Sample Operator : SYSTEM
Acq. Instrument : LCMS-2                      Location  : P2-A5
Injection Date  : 1/5/2024 9:01:32 AM        Inj       :    6
                                           Inj Volume: 2.000 µl

Acq. Method     : C:\Users\Public\Documents\ChemStation\1\Data\010524\010424 2024-01-05 07-
                26-34\PFAA.M
Last changed    : 1/26/2021 10:30:23 AM by SYSTEM
Analysis Method : C:\USERS\PUBLIC\DOCUMENTS\CHEMSTATION\1\METHODS\Purity_195-315.M
Last changed    : 2/6/2023 2:02:18 PM by SYSTEM
Method Info     : OPERATOR: Organic QC lab
                General gradient method starting @100% water for 1 min @0.3 ml/min, the 100
                % Acetonitrile in 13 min, 100% Acetonitrile until T=16 min. Column Zorbax
                Eclipse plus C-18, 2.1mmx50mm, 1.8 µm particle size. Agilent 1290 Infinity
                II LC/MS system, Agilent 6125 quadrupole MS detector.
=====
```

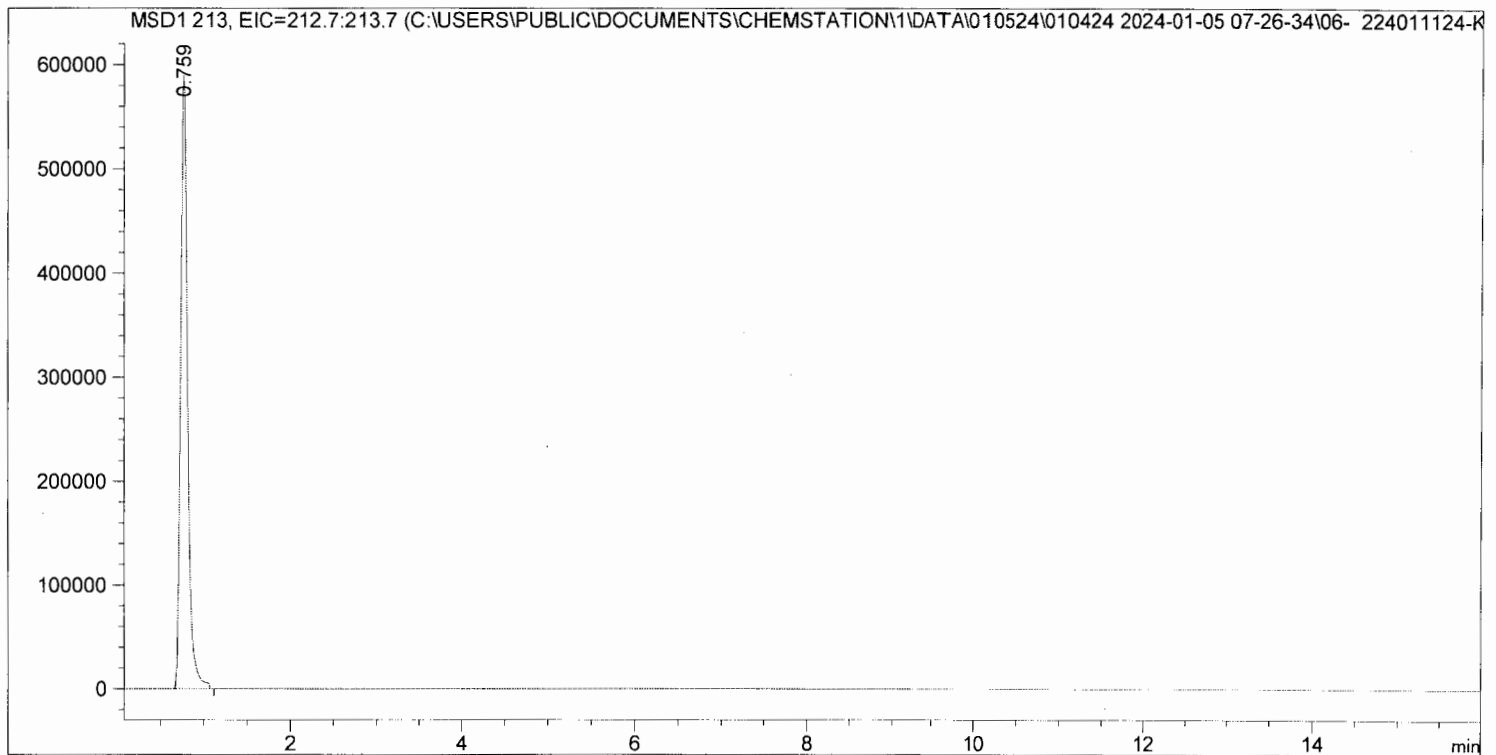

```
=====
                          Area Percent Report
=====
```

```
Sorted By      :      Signal
Multiplier     :      1.0000
Dilution       :      1.0000
Use Multiplier & Dilution Factor with ISTDs
```

Signal 1: MSD1 213, EIC=212.7:213.7


Peak #	RetTime [min]	Type	Width [min]	Area	Height	Area %
1	0.759	BB	0.0891	3.46958e6	5.98649e5	100.0000

Totals : 3.46958e6 5.98650e5

=====  
\*\*\* End of Report \*\*\*



```
=====
Acq. Operator   : SYSTEM                               Seq. Line :    7
Sample Operator : SYSTEM
Acq. Instrument : LCMS-2                               Location  :   P2-A6
Injection Date  : 1/5/2024 9:20:21 AM                 Inj       :    1
                                                    Inj Volume: 2.000 µl
Acq. Method     : C:\Users\Public\Documents\ChemStation\1\Data\010524\010424 2024-01-05 07-
                26-34\PFAA.M
Last changed    : 1/26/2021 10:30:23 AM by SYSTEM
Analysis Method : C:\USERS\PUBLIC\DOCUMENTS\CHEMSTATION\1\METHODS\Purity_195-315.M
Last changed    : 2/6/2023 2:02:18 PM by SYSTEM
Method Info     : OPERATOR: Organic QC lab
                General gradient method starting @100% water for 1 min @0.3 ml/min, the 100
                % Acetonitile in 13 min, 100% Acetonitrile until T=16 min. Column Zorbax
                Eclipse plus C-18, 2.1mmx50mm, 1.8 u particlue size. Agilent 1290 Infinity
                II LC/MS system, Agilent 6125 quadrupole MS detector.
=====
```

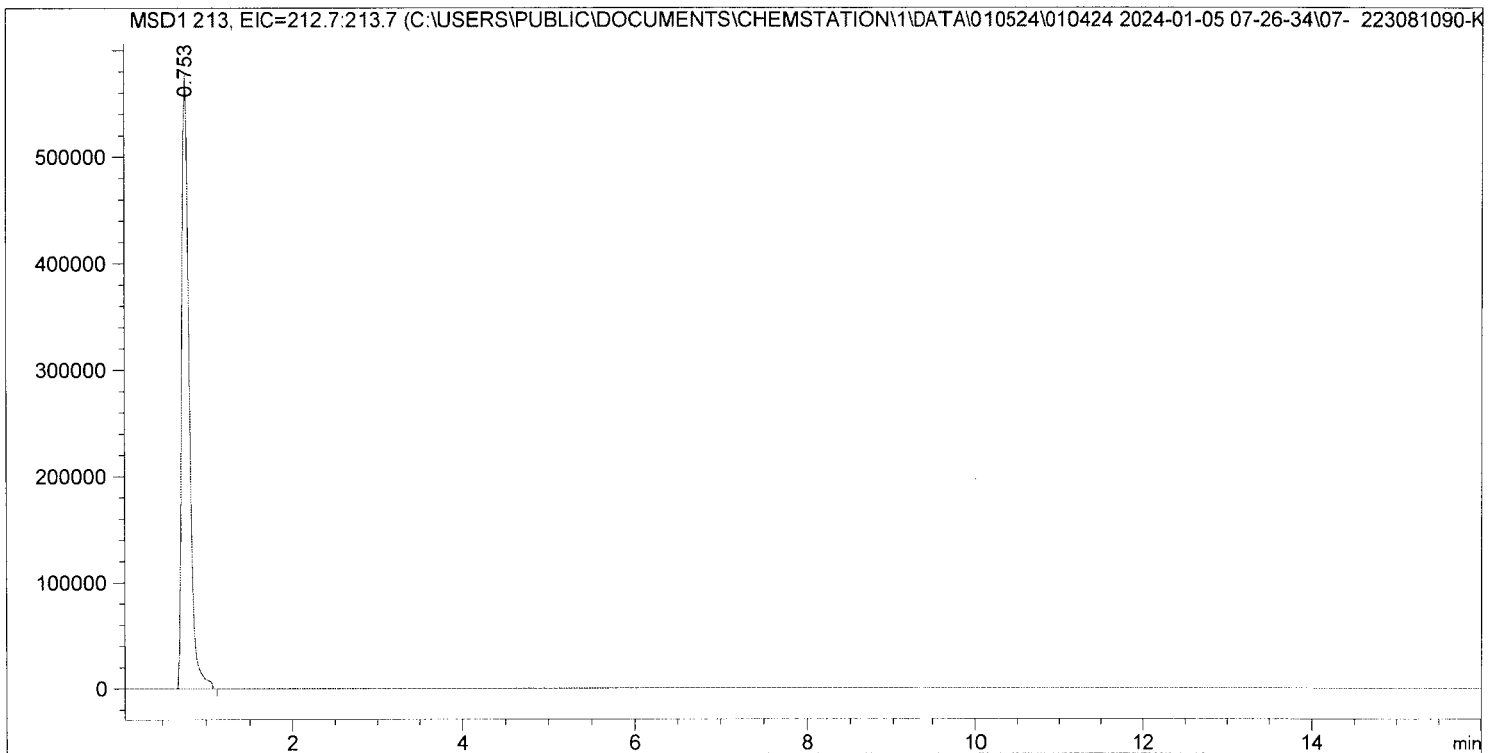

```
=====
                          Area Percent Report
=====
```

```
Sorted By      :      Signal
Multiplier     :      1.0000
Dilution       :      1.0000
Use Multiplier & Dilution Factor with ISTDs
```


Signal 1: MSD1 213, EIC=212.7:213.7

Peak #	RetTime [min]	Type	Width [min]	Area	Height	Area %
1	0.753	BB	0.1008	3.65777e6	5.77582e5	100.0000

Totals : 3.65777e6 5.77582e5

=====  
\*\*\* End of Report \*\*\*

```
=====
Acq. Operator   : SYSTEM                               Seq. Line :    8
Sample Operator : SYSTEM
Acq. Instrument : LCMS-2                               Location  : P2-A6
Injection Date  : 1/5/2024 9:39:10 AM                 Inj       :    2
                                                    Inj Volume: 2.000 µl
Acq. Method     : C:\Users\Public\Documents\ChemStation\1\Data\010524\010424 2024-01-05 07-
                26-34\PFAA.M
Last changed    : 1/26/2021 10:30:23 AM by SYSTEM
Analysis Method : C:\USERS\PUBLIC\DOCUMENTS\CHEMSTATION\1\METHODS\Purity_195-315.M
Last changed    : 2/6/2023 2:02:18 PM by SYSTEM
Method Info     : OPERATOR: Organic QC lab
                General gradient method starting @100% water for 1 min @0.3 ml/min, the 100
                % Acetonitile in 13 min, 100% Acetonitrile until T=16 min. Column Zorbax
                Eclipse plus C-18, 2.1mmx50mm, 1.8 u particlue size. Agilent 1290 Infinity
                II LC/MS system, Agilent 6125 quadrupole MS detector.
=====
```

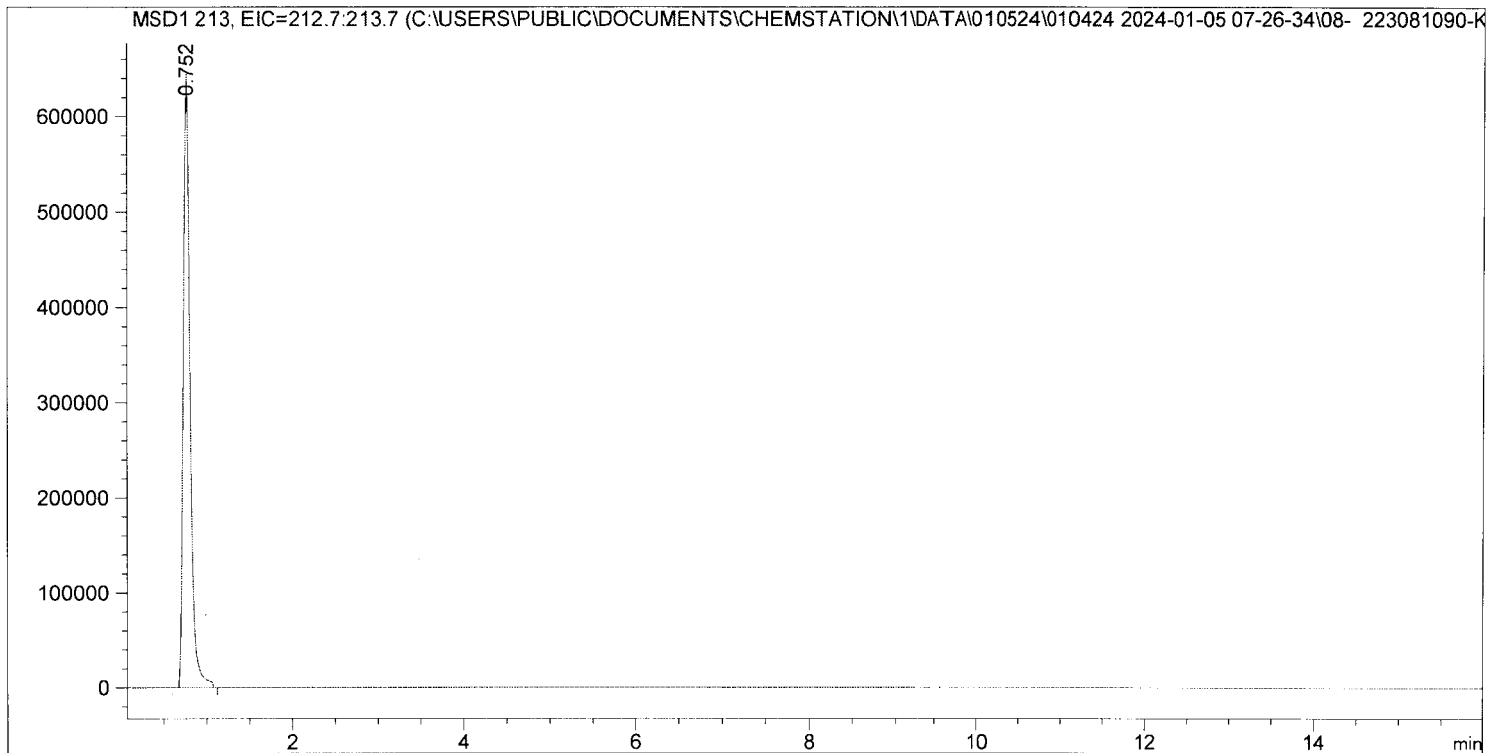

```
=====
                          Area Percent Report
=====
```

```
Sorted By      :      Signal
Multiplier     :      1.0000
Dilution       :      1.0000
Use Multiplier & Dilution Factor with ISTDs
```


Signal 1: MSD1 213, EIC=212.7:213.7

Peak #	RetTime [min]	Type	Width [min]	Area	Height	Area %
1	0.752	BB	0.0893	3.74751e6	6.45405e5	100.0000

Totals : 3.74751e6 6.45405e5

=====  
\*\*\* End of Report \*\*\*

```
=====
Acq. Operator   : SYSTEM                      Seq. Line :    9
Sample Operator : SYSTEM
Acq. Instrument : LCMS-2                      Location  :   P2-A6
Injection Date  : 1/5/2024 9:57:59 AM        Inj       :    3
                                           Inj Volume: 2.000 µl
Acq. Method     : C:\Users\Public\Documents\ChemStation\1\Data\010524\010424 2024-01-05 07-
                26-34\PFAA.M
Last changed    : 1/26/2021 10:30:23 AM by SYSTEM
Analysis Method : C:\USERS\PUBLIC\DOCUMENTS\CHEMSTATION\1\METHODS\Purity_195-315.M
Last changed    : 2/6/2023 2:02:18 PM by SYSTEM
Method Info     : OPERATOR: Organic QC lab
                General gradient method starting @100% water for 1 min @0.3 ml/min, the 100
                % Acetonitrile in 13 min, 100% Acetonitrile until T=16 min. Column Zorbax
                Eclipse plus C-18, 2.1mmx50mm, 1.8 µm particle size. Agilent 1290 Infinity
                II LC/MS system, Agilent 6125 quadrupole MS detector.
=====
```

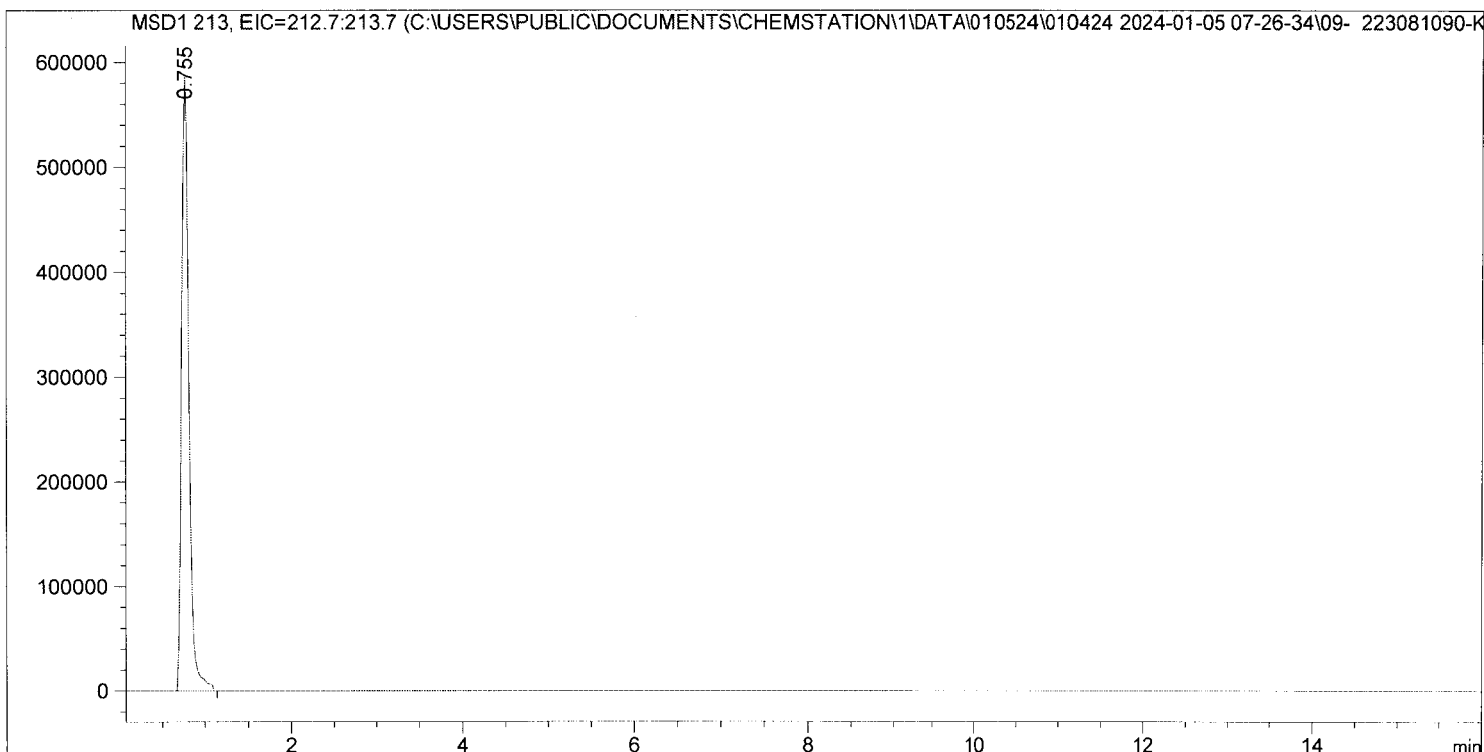

=====  
Area Percent Report  
=====

```
Sorted By      :      Signal
Multiplier     :      1.0000
Dilution       :      1.0000
Use Multiplier & Dilution Factor with ISTDs
```

Signal 1: MSD1 213, EIC=212.7:213.7

Peak #	RetTime [min]	Type	Width [min]	Area	Height	Area %
1	0.755	BB	0.0963	3.49319e6	5.87523e5	100.0000

Totals : 3.49319e6 5.87523e5

=====  
\*\*\* End of Report \*\*\*



Totals : 3.67844e6 6.26437e5

=====  
\*\*\* End of Report \*\*\*





Totals : 3.21351e6 5.45953e5

=====  
\*\*\* End of Report \*\*\*