Print of window 38: Current Chromatogram(s)
Data File : D:\DATA\11132023\21- KM.D
Sample Name : M-8330B-R-10X

==========

Acq. Operator : SYSTEM Seq. Line : 3
Acq. Instrument : LCMS-1 Location : P1-D4
Injection Date : 11/13/2023 4:57:48 PM Inj : 2
Inj Volume : 1.000 µl

Acq. Method : C:\CHEM32\1\METHODS\ExplosivesPT_10C.M
Last changed : 7/20/2021 1:26:52 PM by SYSTEM
Analysis Method : C:\CHEM32\1\METHODS\Purity195_315.M
Last changed : 11/13/2023 1:56:31 PM by SYSTEM
(modified after loading)
Method Info : Operator: Organic QC lab
Gradient Method Starting @ 100 % Water/0 % Acetonitrile to 0 % Water/100 % Acetonitrile in 13 min, then 3 min at 100/0, post-run time 2 min. Flow rate:0.3 ml /min, column Zorbax Eclipse Plus C-18, 2.1x50 mm, 1.8 micron particle size. Agilent 1290 Infinity II LC system, Agilent 6120 Quadrople MS Detector. No UV Reference.

Sample Info : Explosives by HPLC in 50:50 ACN/MeOH

Additional Info : Peak(s) manually integrated
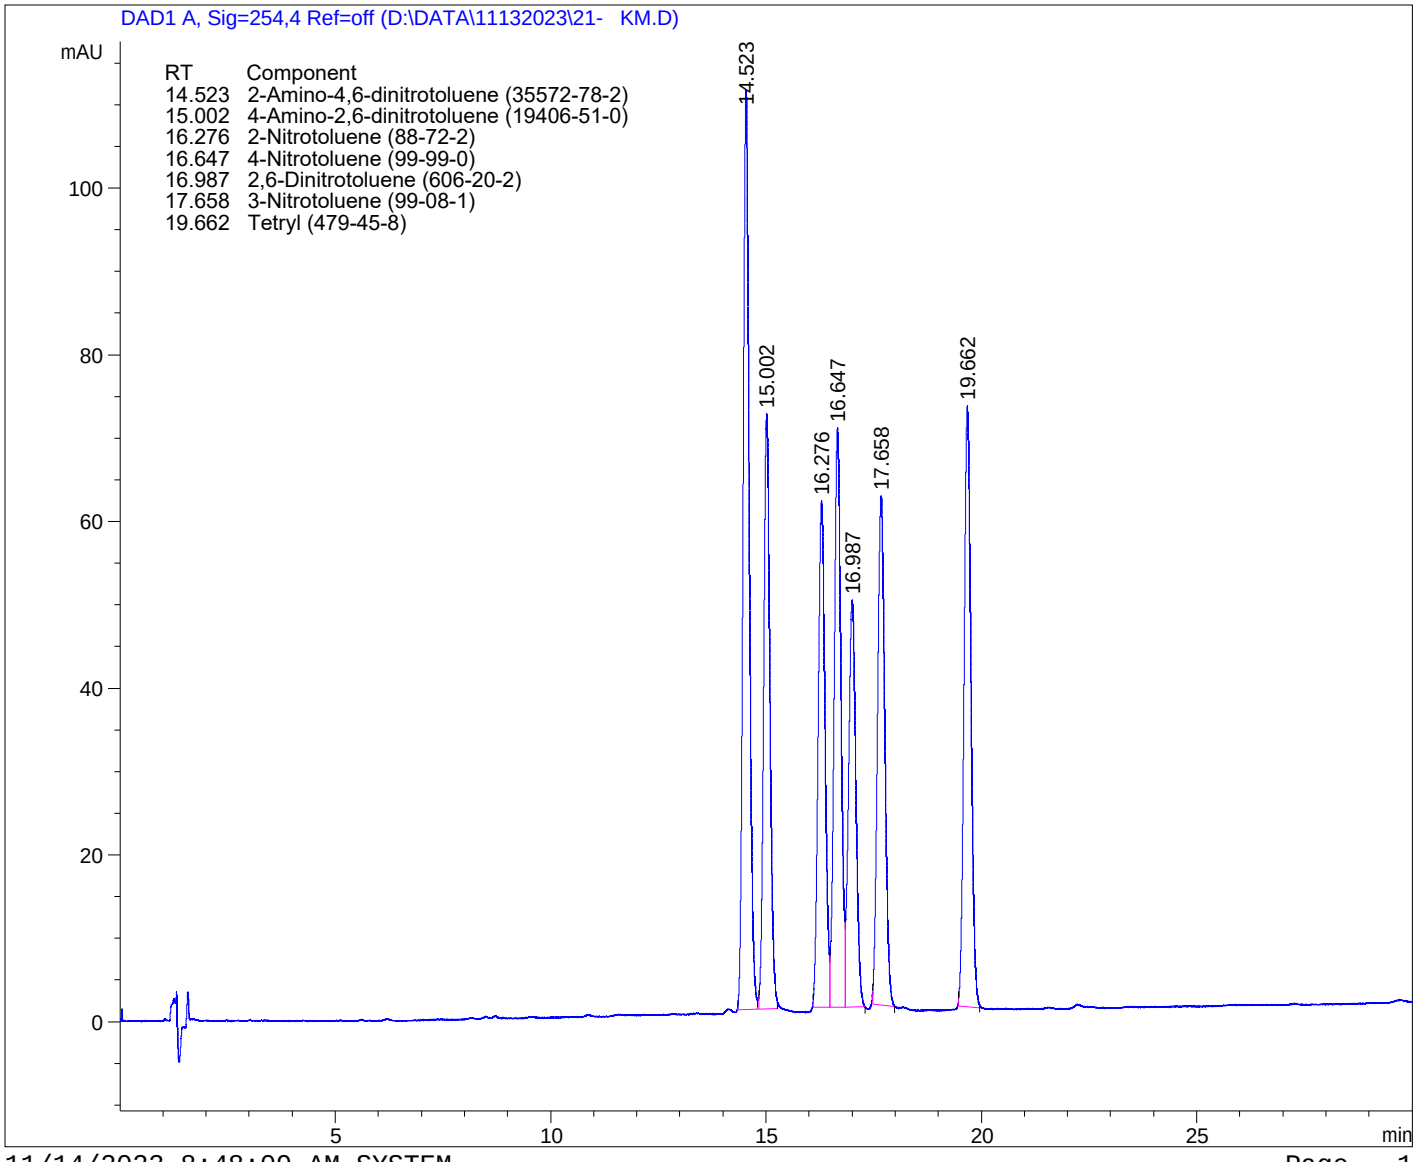
Current Chromatogram(s)