


File :Q:\GCMS-04\DATA\030419\21-.D
 Operator : RFXM
 Acquired : 5 Mar 19 1:15 am using AcqMethod VOC-SCAN 24 DECKER.M
 Instrument : GCMS4
 Sample Name: M-GRO-CAL-IS-05-R1
 Misc Info :
 Vial Number: 46



Column: DB-624 UI, 30m x 0.25mm ID x 1.4µm
 Oven Program: 35°C (hold 5min), 11°C/min to 60°C, 22°C/min to 230°C (hold 4min)
 GC Parameters: Split 100:1, 1µl inj.; GC/MS; Injector temp 240°C

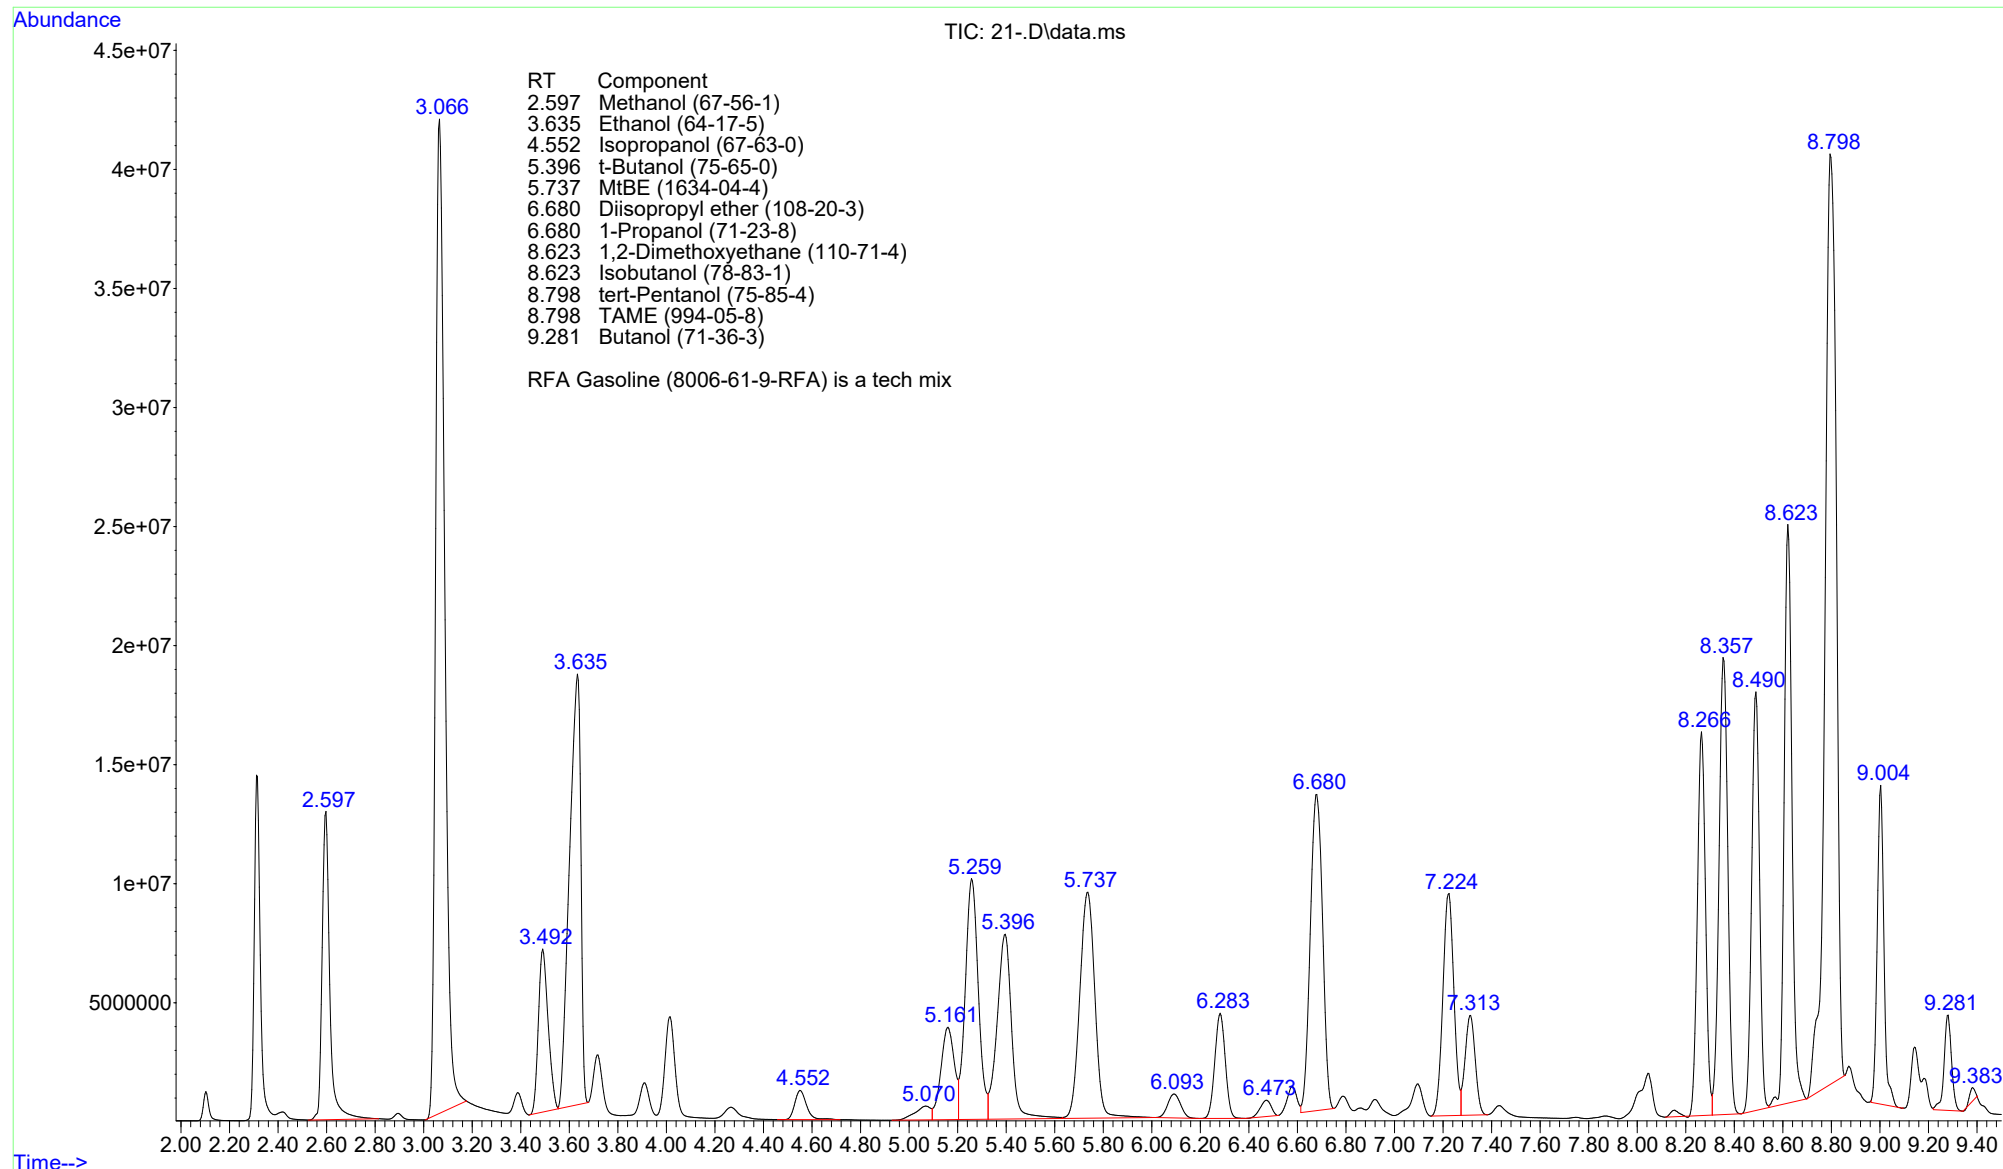

Not in mix - EtBE (637-92-3), sec-Butanol (78-92-2)