

# AccuStandard®

Sample Name: P-093-WL-5X-5ML

File: C:\CPData\DATA\2022\0714\222071202 JP(1).0000.RAW

Date (start): 7/14/2022 12:06:53 PM

Column: 11m, 0mL, 160/min to 326, Final 2 min

Parameters: Splitless; 2u; ECD: 325c; Inj: 250c

notes:

Method: NL\_FAST\_ECD.MET


Setpoint File: NL\_FAST\_ECD.M68

Calibration File:

Inst: GC#7

Oper: JJP

Vol = 2

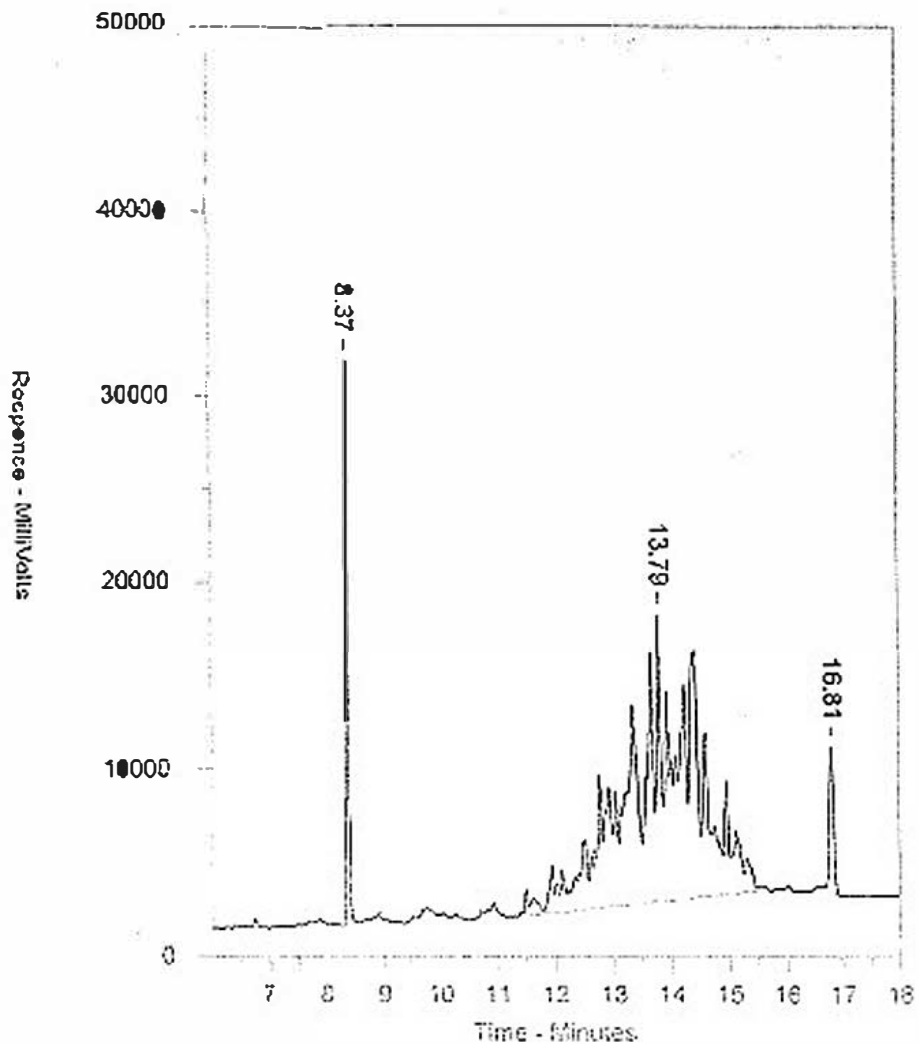

8.37	Tetrachloro-meta-xylene (877-09-8)
13.78	Toxaphene (8001-35-2)
16.80	Decachlorobiphenyl (2051-24-3)