Print of window 38: Current Chromatogram(s)
Data File : D:\DATA\04041901\04041901 2019-04-04 06-53-00\03- .D
Sample Name : P-402S

==========

Acq. Operator : SYSTEM Seq. Line : 3
Acq. Instrument : LCMS-1 Location : P1-D2
Injection Date : 4/4/2019 7:30:58 AM Inj : 1
Inj Volume : 1.000 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 0.100 µl
Acq. Method : D:\DATA\04041901\04041901 2019-04-04 06-53-00\Purity195_315.M
Last changed : 4/4/2019 6:53:00 AM by SYSTEM
Analysis Method : C:\CHEM32\1\METHODS\Purity195_315.M
Last changed : 6/6/2017 9:45:25 AM by SYSTEM
Method Info : Operator: GA
Gradient Method Starting @ 100 % Water/0 % Acetonitrile to 0 % Water/100 % Acetonitrile in 13 min, then 3 min at 100/0, post-run time 2 min. Flow rate:0.3 ml /min, column Zorbax Eclipse Plus C-18, 2.1x50 mm, 1.8 micron particule size. Agilent 1290 Infinity II LC system, Agilent 6120 Quadrople MS Detector. No UV Reference.

Sample Info : Chloroxuron

Additional Info : Peak(s) manually integrated
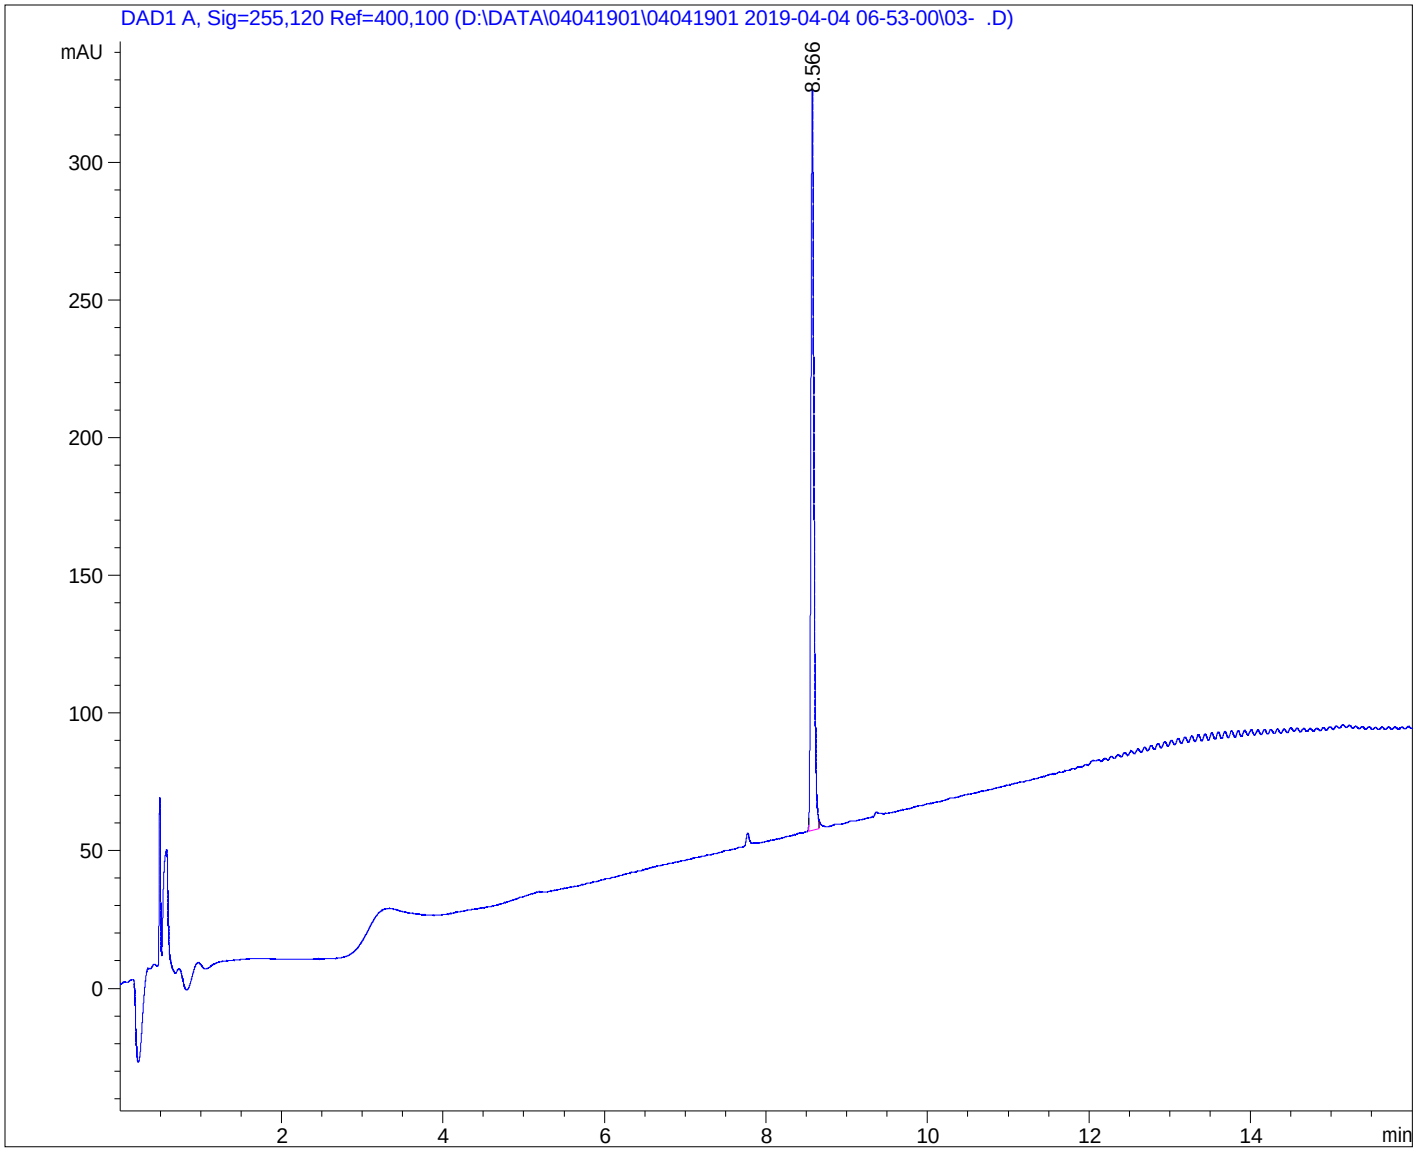
Current Chromatogram(s)