Print of window 38: Current Chromatogram(s)
Data File : D:\DATA\09172001\01--GA.D
Sample Name : P-632S

Acq. Operator	: SYSTEM	Seq. Line	: 1
Acq. Instrument	: LCMS-1	Location	: P2-B7
Injection Date	: 9/17/2020 10:11:21 AM	Inj	: 1
		Inj Volume	: 1.000 µl
Method	: C:\CHEM32\1\METHODS\Purity195_315.M		
Last changed	: 5/8/2020 11:20:44 AM by SYSTEM		
Method Info	: Operator: Oraganic QC lab Gradient Method Starting @ 100 % Water/0 % Acetonitrile to 0 % Water/100 % Acetonitrile in 13 min, then 3 min at 100/0, post-run time 2 min. Flow rate:0.3 ml /min, column Zorbax Eclipse Plus C-18, 2.1x50 mm, 1.8 micron particule size. Agilent 1290 Infinity II LC system, Agilent 6120 Quadrople MS Detector. No UV Reference.		
Additional Info	: Peak(s) manually integrated		
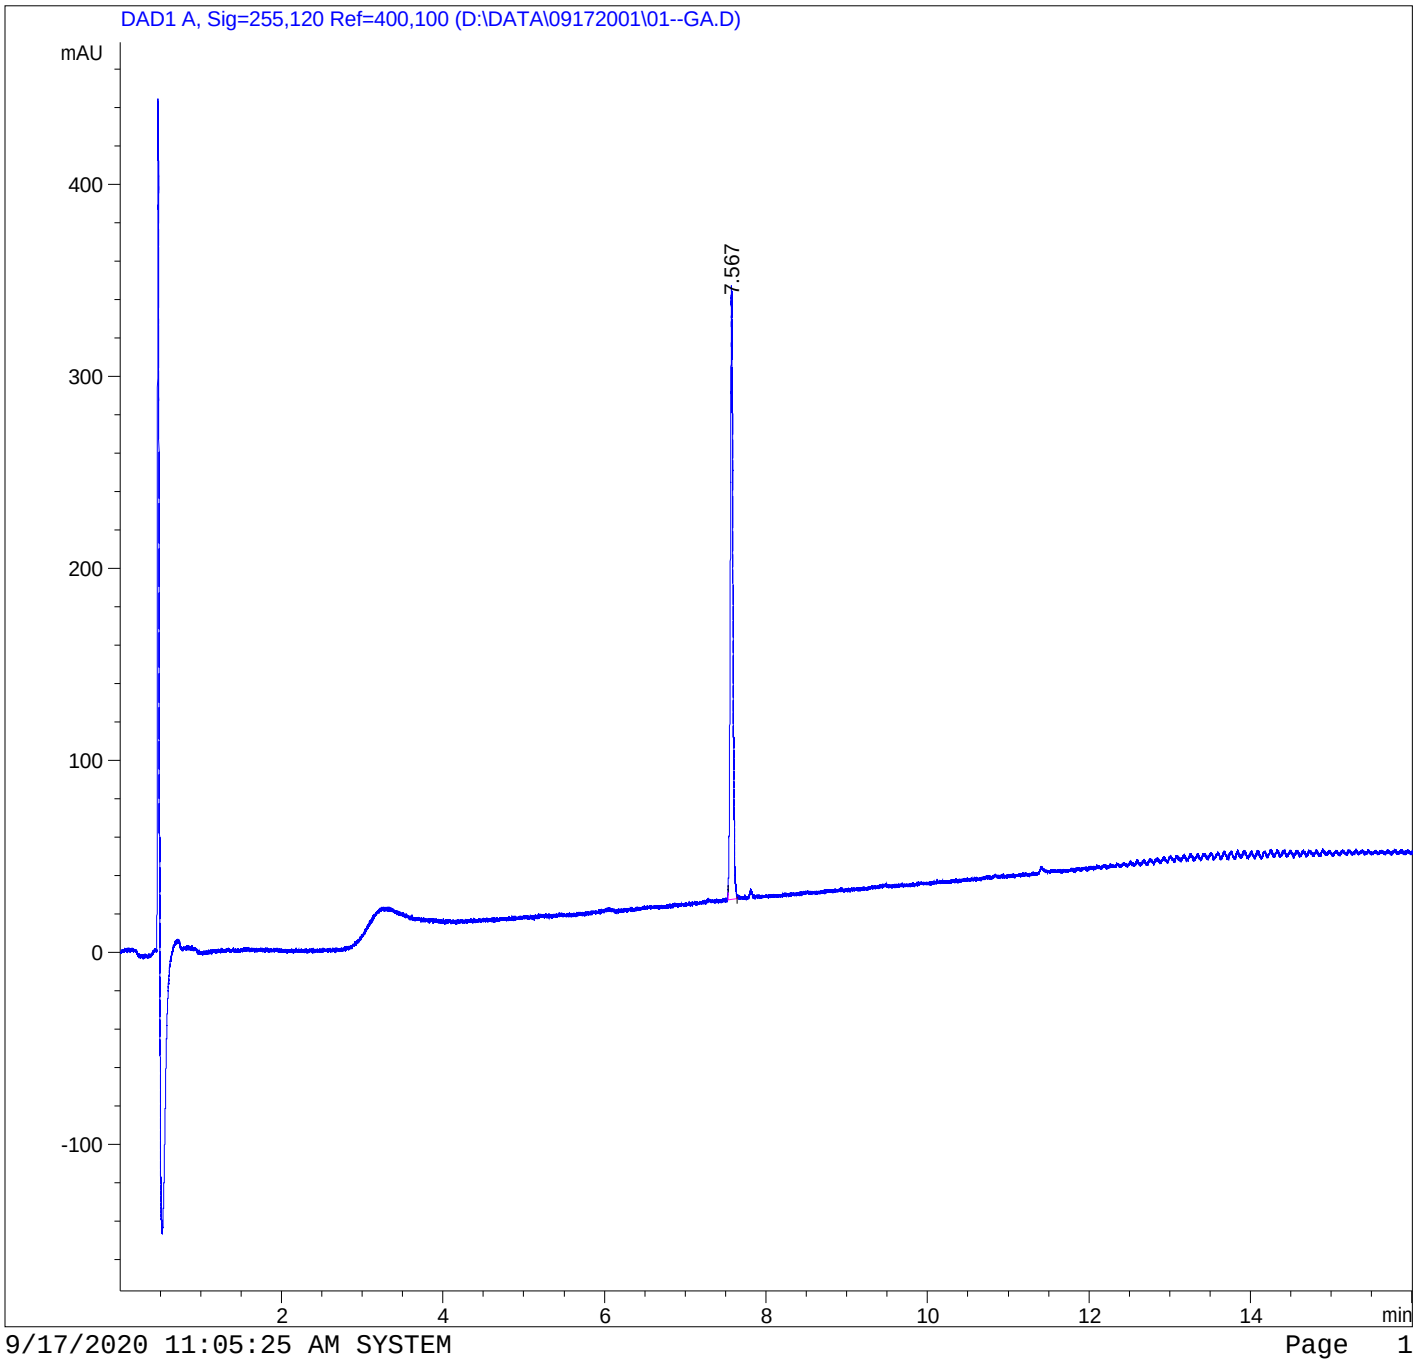
Current Chromatogram(s)