Print of window 38: Current Chromatogram(s)
Data File : D:\DATA\11042021\02- KM.D
Sample Name : P-962S-CN (221111084)

==========

Acq. Operator : SYSTEM
Seq. Line : 2
Acq. Instrument : LCMS-1
Location : P1-C4
Injection Date : 11/4/2021 1:22:54 PM
Inj : 2
Inj Volume : 1.000 µl

Acq. Method : C:\CHEM32\1\METHODS\Purity195_315.M
Last changed : 10/29/2021 2:16:13 PM by SYSTEM
Analysis Method : C:\CHEM32\1\METHODS\Purity195_315.M
Last changed : 10/8/2021 11:40:47 AM by SYSTEM
Method Info : Operator: Organic QC lab
Gradient Method Starting @ 100 % Water/0 % Acetonitrile to 0 % Water/100 % Acetonitrile in 13 min, then 3 min at 100/0, post-run time 2 min. Flow rate :0.3 ml/min, column Zorbax Eclipse Plus C-18, 2.1x50 mm, 1.8 micron particle size. Agilent 1290 Infinity II LC system, Agilent 6120 Quadrople MS Detector. No UV Reference.

Sample Info : Mesotrione @ 100 ug/mL in AcCN

Additional Info : Peak(s) manually integrated
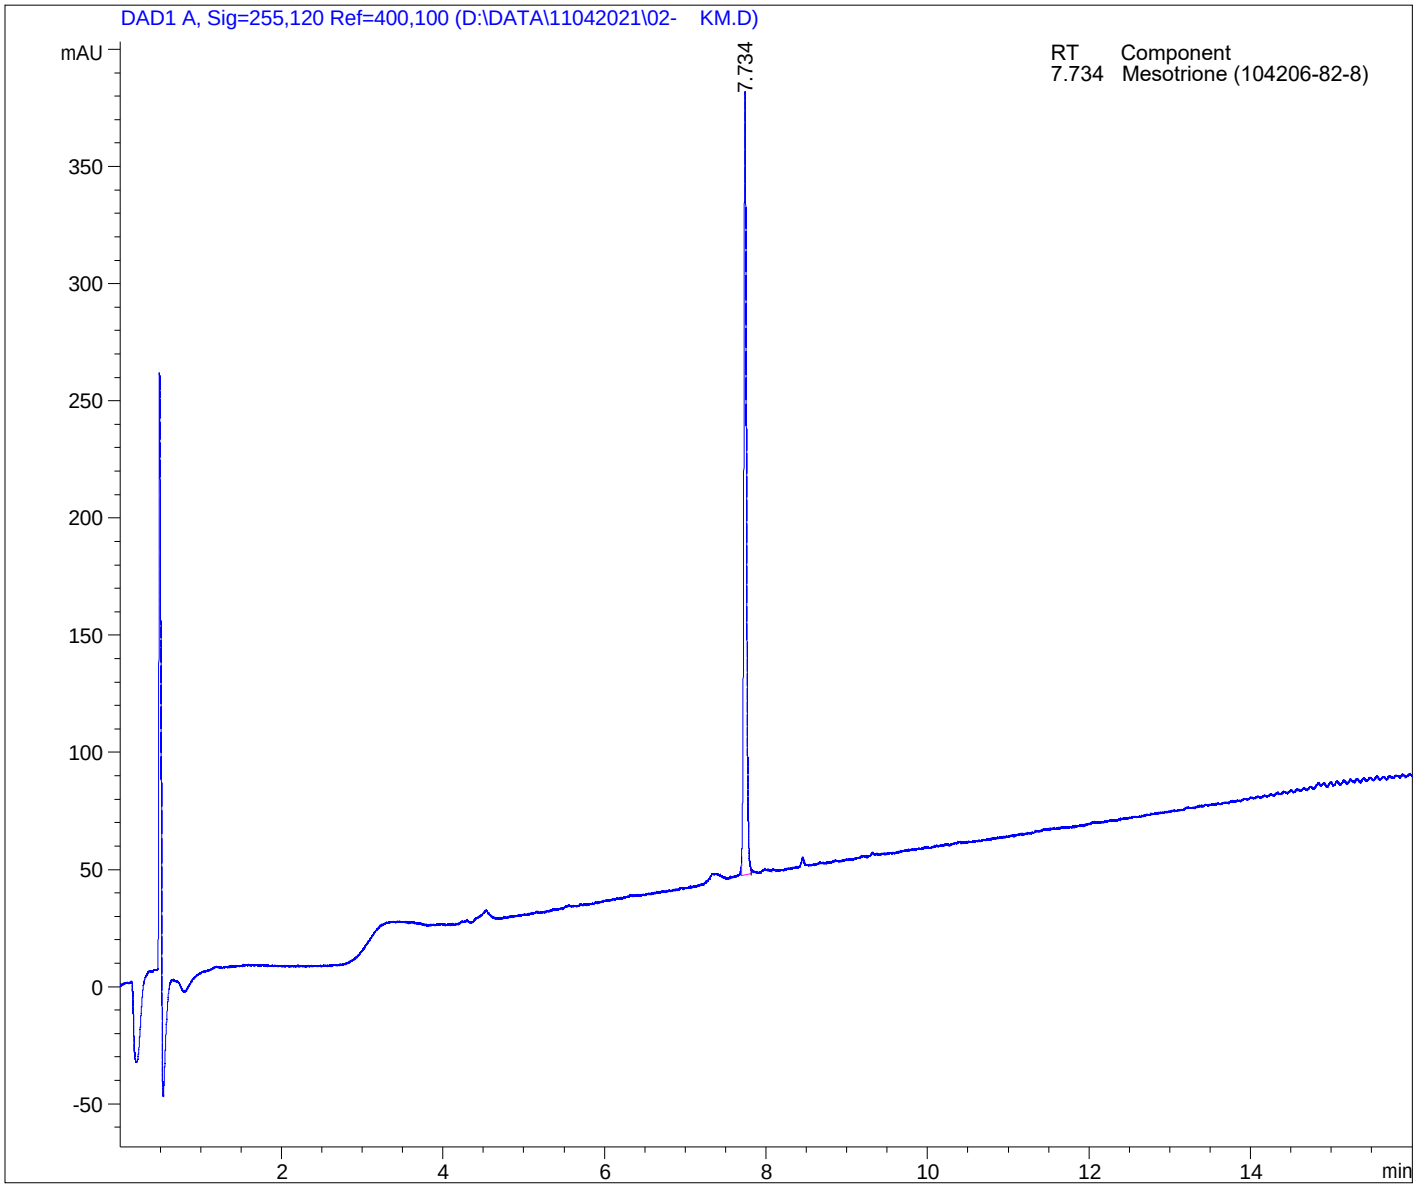
Current Chromatogram(s)