Print of window 38: Current Chromatogram(s)
Data File : C:\USERS\P...ON\1\DATA\06072201\06072201 2022-06-07 06-39-34\45- -KD.D
Sample Name : PFOA-015S-0.02X

==========

Acq. Operator : SYSTEM Seq. Line : 45
Sample Operator : SYSTEM
Acq. Instrument : LCMS-2 Location : P1-A1
Injection Date : 6/7/2022 8:32:26 PM Inj : 3
Inj Volume : 2.000 µl
Different Inj Volume from Sample Entry! Actual Inj Volume : 1.000 µl
Acq. Method : C:\Users\Public\Documents\ChemStation\1\Data\06072201\06072201 2022-06-07 06-39-34 \PFAA.M
Last changed : 1/26/2021 10:30:23 AM by SYSTEM
Analysis Method : C:\USERS\PUBLIC\DOCUMENTS\CHEMSTATION\1\METHODS\Purity_195-315.M
Last changed : 5/16/2022 12:35:31 PM by SYSTEM
(modified after loading)
Method Info : OPERATOR: Organic QC lab
General gradient method starting @100% water for 1 min @0.3 ml/min,the 100% Acetonitile in 13 min, 100% Acetonitrile until T=16 min. Column Zorbax Eclipse plus C-18, 2.1mmx50mm, 1.8 u particlue size. Agilent 1290 Infinity II LC/MS system , Agilent 6125 quadrupole MS detector.
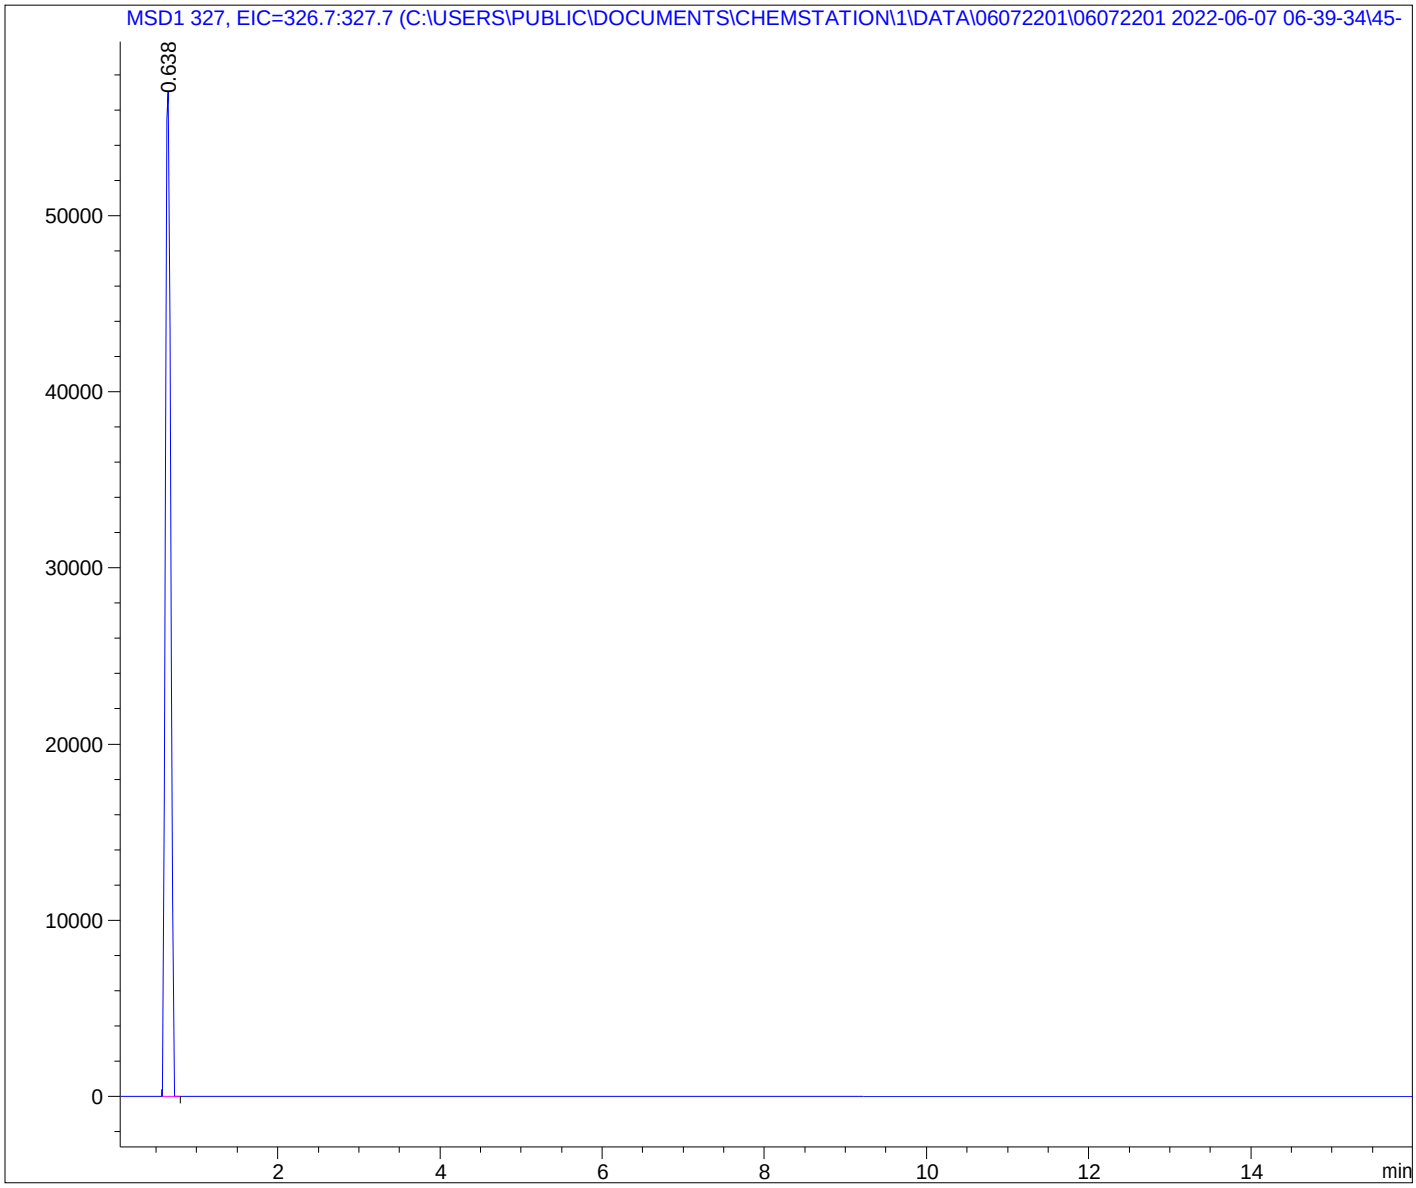
Current Chromatogram(s)