Print of window 38: Current Chromatogram(s)
Data File : D:\DATA\10182021\08-KD.D
Sample Name : PLAS-UV-11S-CN

AccuStandard®
Leader in Analytical Reference Standards

==========

Acq. Operator : SYSTEM Seq. Line : 2
Acq. Instrument : LCMS-1 Location : P1-D4
Injection Date : 10/18/2021 12:24:42 PM Inj : 2
Inj Volume : 1.000 µl

Method : C:\CHEM32\1\METHODS\POS_NEG_50_50_GRAD0-100.M
Last changed : 2/26/2018 2:30:50 PM by SYSTEM
Method Info : Operator: GA
Gradient Method Starting @ 100 % Water/0 % Acetonitrile to 0 % Water/100 % Acetonitrile in 13 min, then 3 min at 100/0, post-run time 2 min. Flow rate:0.3 ml /min, column Zorbax Eclipse Plus C-18, 2.1x50 mm, 1.8 micron particule size. Agilent 1290 Infinity II LC system, Agilent 6120 Quadrople MS Detector. No UV Reference.

Additional Info : Peak(s) manually integrated
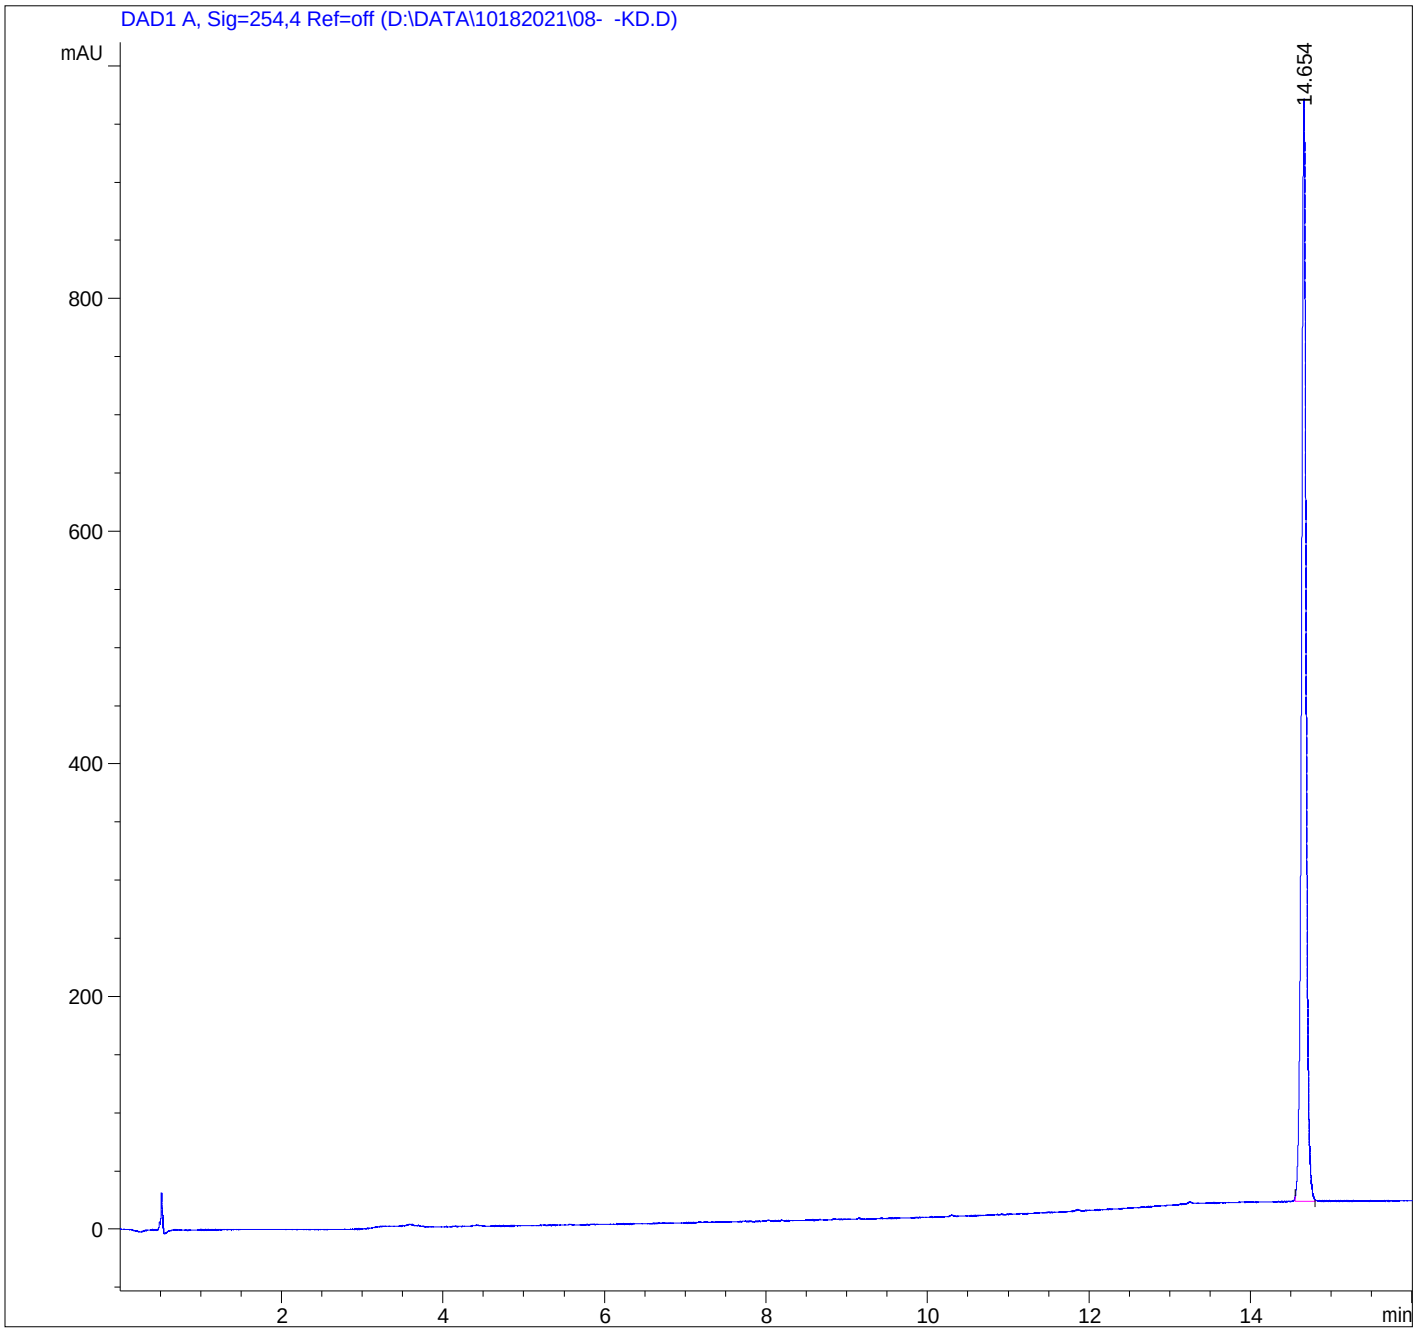
Current Chromatogram(s)